




## TaiDoc TD-1242 Forehead Thermometer Instruction Manual

[Home](#) » [TaiDoc](#) » TaiDoc TD-1242 Forehead Thermometer Instruction Manual 


# TaiDoc

TD-1242  
Forehead Thermometer  
Operation Instructions

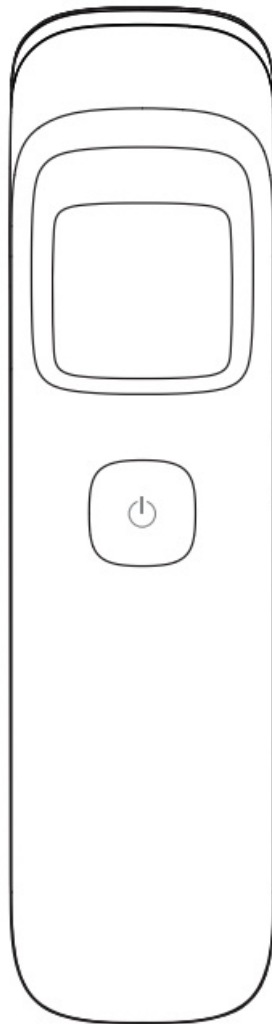

311-1242100-012  
Version 1.0 2020/02

 MedNet GmbH

 Borkstrae 10, 48163 Münster – Germany  
TaiDoc Technology Corporation  
B1-7F, No. 127, Wugong 2nd Rd., Wugu Dist.,  
24888 New Taipei City, Taiwan  
[www.taidoc.com](http://www.taidoc.com)




## **Contents**

- [1 APPEARANCE AND KEY FUNCTIONS](#)
- [2 INTRODUCTION](#)
- [3 IMPORTANT SAFETY INSTRUCTIONS](#)
- [4 CAUTIONS AND WARNINGS](#)
- [5 HOW TO USE](#)
- [6 INSTALL BATTERY](#)
- [7 MEASURING TEMPERATURES-  
GENERALS](#)
- [8 MEASURING TEMPERATURES-CHILDREN](#)
- [9 MEASURING TEMPERATURES-SURFACE](#)
- [10 CHANGING UNIT OF MEASUREMENT](#)
- [11 RECALLING PAST READINGS](#)
- [12 NORMAL BODY TEMPERATURE &  
FEVER](#)
- [13 MAINTENANCE](#)
- [14 TROUBLESHOOTING](#)
- [15 SYMBOL INFORMATION](#)
- [16 SPECIFICATIONS](#)
- [17 REFERENCE STANDARDS](#)
- [18 Documents / Resources](#)
- [19 Related Posts](#)

## **APPEARANCE AND KEY FUNCTIONS**

1. Display Screen
2. Power / Scan Button
3. Probe
4. Mode Button
5. Memory Button
6. Battery Cover 4

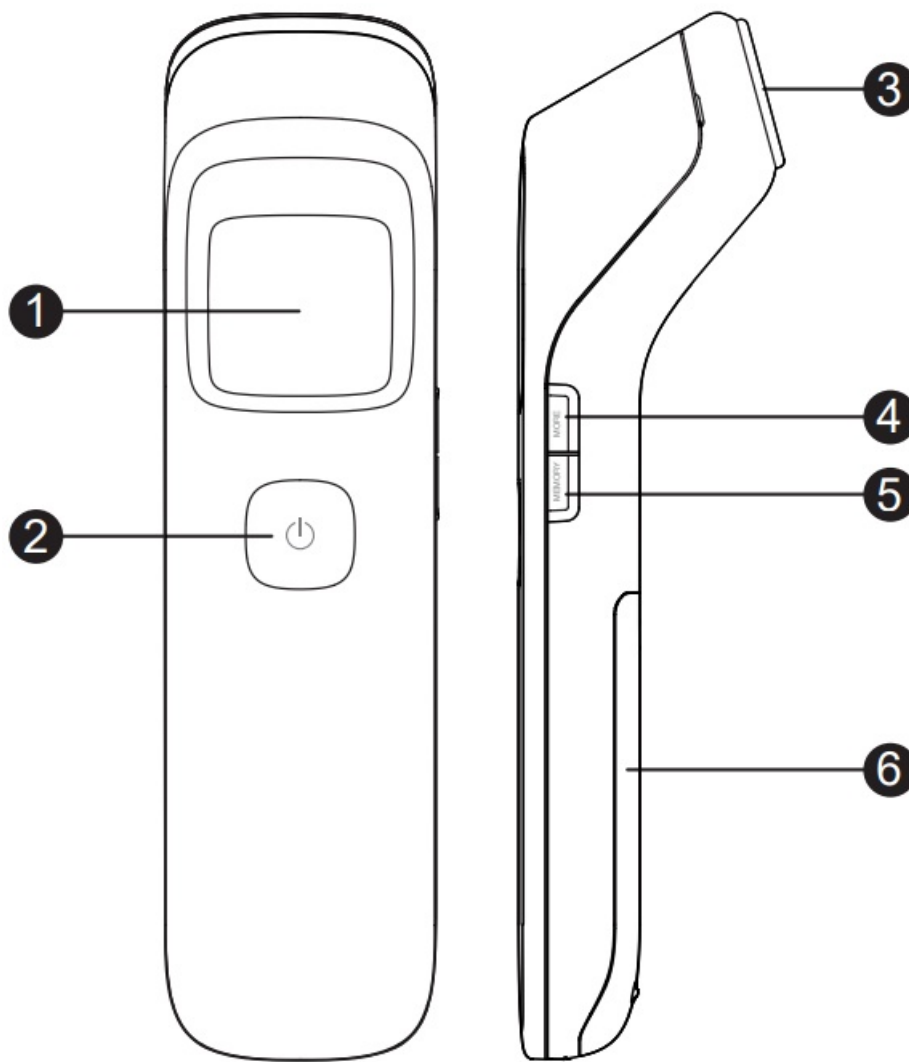

## INTRODUCTION

Thank you for choosing the TD-1242 Forehead Thermometer. Please read this instruction manual first so you can use this thermometer safely and correctly. Please keep this instruction manual for future reference. This innovative medical device uses advanced infrared (IR) technology to measure temperature instantly and accurately on the forehead/surface. The TD-1242 Forehead Thermometer delivers a body temperature reading from the thermal radiation emitted from the forehead without contact with the body. (The surface temperature measurement is not for medical purposes.) Before using this product, please read the following contents thoroughly and carefully.

### INTENDED USE

The TD-1242 forehead thermometer is intended for the intermittent measurement and monitoring of human body temperature from the forehead. The device is intended for use of all ages for home and professional use by one with a good understanding of the operation instruction, where the patient may be an operator.

### HOW DOES IT WORK

The thermometer measures the infrared heat generated by the surface of the skin over the vessel and its surrounding tissue. The thermometer then converts it into a temperature value shown on LCD.

## IMPORTANT SAFETY INSTRUCTIONS

### READ THIS BEFORE USING AND KEEP THESE INSTRUCTIONS

1. Close supervision is necessary when the thermometer is used by, on, or near children, handicapped persons, or invalids.
2. Use the thermometer only for the intended use described in this manual.


3. Do not use the thermometer if it is not working properly, or if it has sustained any damage.
4. Keep the sensor end clean and free of debris. See Maintenance section for instructions.
5. Do not use ethylene oxide gas, heat, autoclave, or any other harsh methods to sterilize the device.
6. If coming from an environment of warmer or cooler temperature or after a period of exertion, allow the user and the thermometer to acclimate to room temperature for 20 minutes prior to taking a measurement.
7. As the forehead temperature may be affected by sweat, oil, and the surrounding temperature, the reading shall be taken as a reference only.
8. Do not use in presence of flammable anesthetic mixtures.
9. Do not use accessories that are not supplied or recommended by the manufacturer. Do not try to modify the device to prevent any dangers.
10. Proper maintenance is essential to the longevity of your device. If you are concerned about the accuracy of measurement, please contact the local customer service or place of purchase for help.
11. Always contact the manufacturer or the manufacturer's representative to report unexpected operations or events. Do not try to fix it by yourself.
12. When using the thermometer, stay away from electromagnetic radiation, such as the mobile in use.
13. Do not expose the device to strong electrostatic fields or strong magnetic fields to avoid affecting the measurement accuracy.
14. Used in close proximity to others, EMC must be tested and verified.
15. The small parts detached from the device may result in children choking from inhaling or swallowing.
16. Do not try to maintain the device while it is in use.
17. This thermometer has been calibrated at the factory. If you follow the instructions, you don't need to adjust them regularly. But if you are in doubt about the accuracy of the readings, please contact customer service.

## **CAUTIONS AND WARNINGS**

- Always operate the thermometer in an operating temperature range 10°C to 40°C (50°F to 104°F), and relative humidity 30% to 85%.
- Always store the thermometer in a cool and dry place: temperatures between -20°C to 60°C (-4°F to 140°F); relative humidity 30% to 85%. Avoid direct sunlight.
- Avoid dropping the thermometer.
- This thermometer is not intended to be a substitution for a consultation with your physician.

## **LCD SCREEN**


1. Temperature display
2. Error message
3. Memory mode
4. Hold Symbol
5. Temperature unit
6. Battery indicator
7. General body temperature indicator
8. Child body temperature indicator 9 Object surface temperature indicator

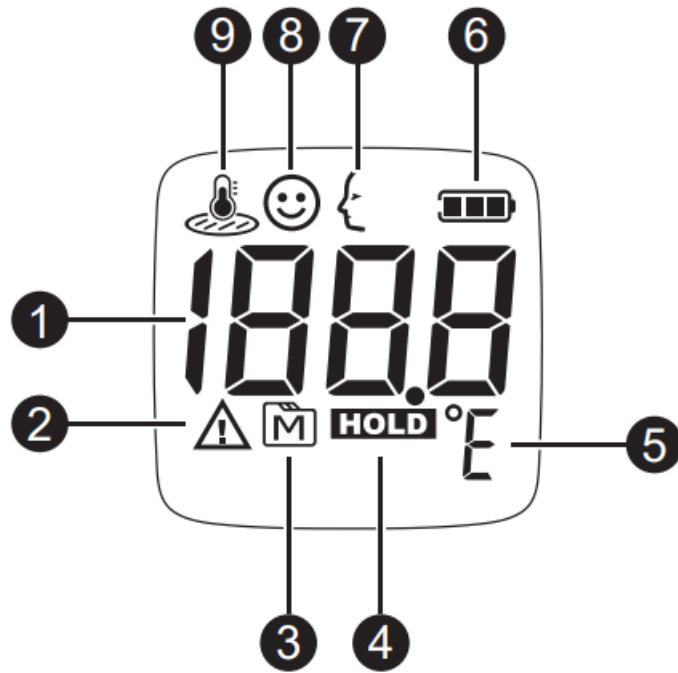


## HOW TO USE

### INSTALL BATTERY

1. Remove the battery cover by pressing down at the arrow mark and slide in the direction of the arrow (Figure 1).
2. Install (2) AAA alkaline batteries and close the battery cover (Figure 2).
3. If the thermometer will be stored without use, remove batteries.

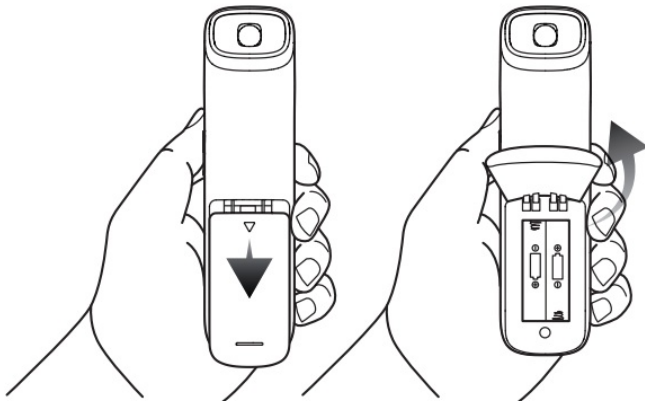

( Figure 1 )

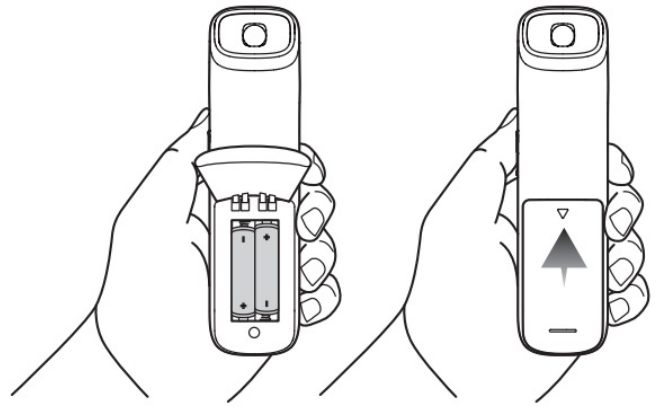

( Figure 2 )

### Warning:

Make sure the battery cover is properly closed and secured.


### MEASURING TEMPERATURES-GENERALS

(older than 36 months)

1. The forehead should be clear of hair and perspiration.
2. Aim at the center forehead area 3 to 7cm (1" to 2.5") away from the skin surface. Be sure the thermometer is perpendicular to the skin surface.



3. Press and release the SCAN button to take a measurement. A double “beep” sound indicates a reading has been taken and displayed on the LCD screen. When a reading is greater than 38.0°C, a warning symbol will flash with Red backlight.

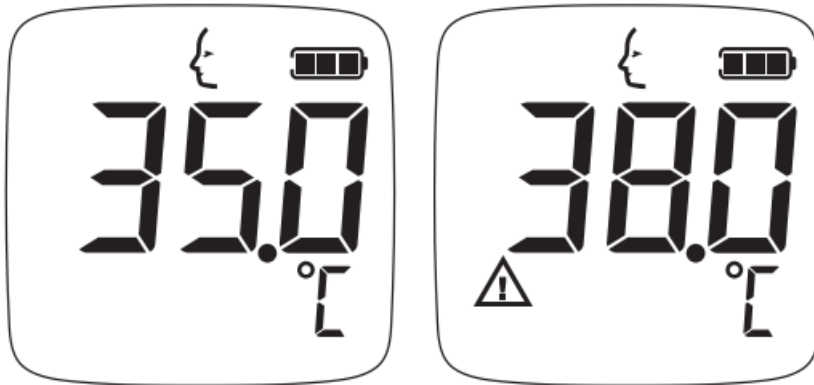

4. To take another measurement, follow steps 2 and 3.
5. The thermometer turns off automatically after 30 seconds.


**NOTE:**

- If the reading is 31.9°C (89.5°F), the display will show “Lo”.
- If the reading is 32.0°C (89.6°F) and 37.9 °C (100.3°F), the display will show the reading with green backlight.
- If the reading is 38.0 °C (100.4°F) and 43°C (109.4°F), the display will show the reading with red backlight.
- If the reading is 43.1°C (109.5°F), the display will show “Hi”.


**MEASURING TEMPERATURES-CHILDREN**

**(younger than 36 months)**

1. Press the SCAN button to turn on the thermometer.
2. Press and hold the MODE button for 1 second before releasing. A general facial profile should be flashing, indicating that the preset mode is for generals.
3. Press the MODE key to switch to Child mode, indicated by a smiley face icon.

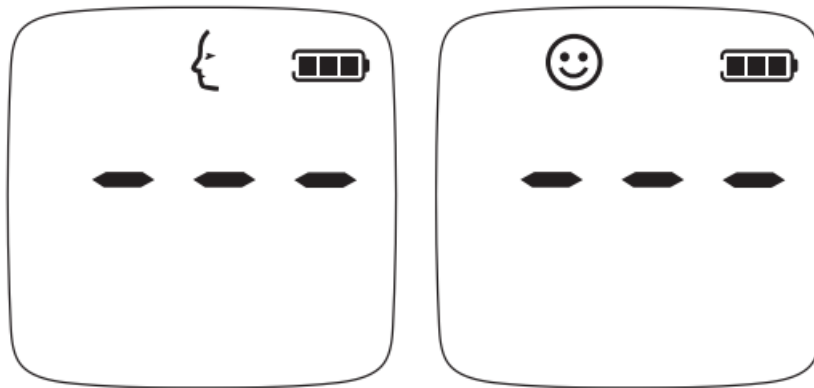

4. Aim the scanner at the center of the child's forehead 3 to 7cm (1" to 2.5") away from the skin surface. Press and release the SCAN button to take a measurement. A red backlight with a warning symbol indicates a reading greater than 37.6 °C (99.7°F).

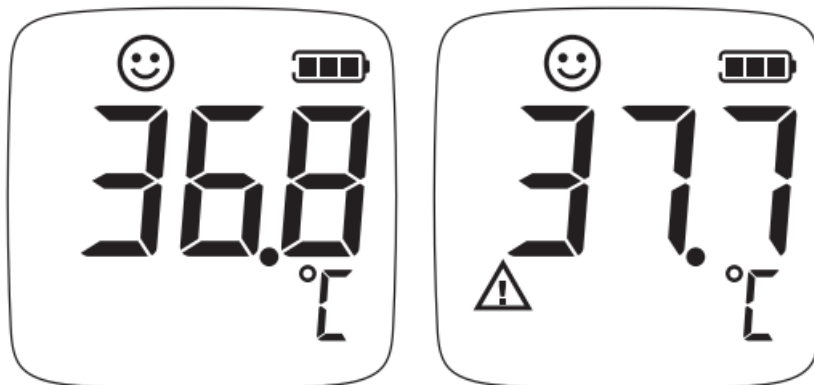


5. The thermometer automatically switches off when left idle for 30 seconds.

#### NOTE:


- If the reading is 31.9°C (89.5°F), the display will show "Lo".
- If the reading is 32°C (89.6°F) and 37.6 °C (99.7°F), the display will show the reading with green backlight.
- If the reading is 37.7 °C (99.8°F) and 43°C (109.4°F), the display will show the reading with red backlight.
- If the reading is 43.1°C (109.5°F), the display will show "Hi".

#### MEASURING TEMPERATURES-SURFACE

1. Press the SCAN button to turn on the thermometer.
2. Press and hold the MODE button for 1 second before releasing. A general facial profile should be flashing, indicating that the preset mode is for generals.
3. Press the MODE key to switch to Surface mode, indicated by a thermometer icon.

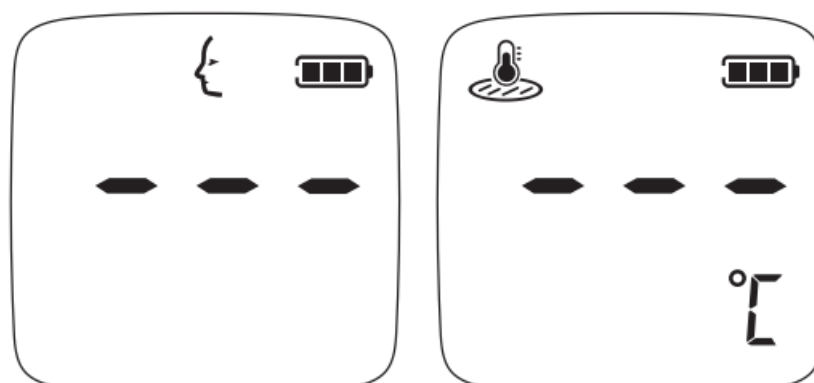

4. Press the SCAN button. Make sure the probe is flat and close to the object's surface, not at an angle. Perform an object measurement with a distance within 5 cm (1.9 inches). Press and hold the SCAN button as you move the meter along the surface. The HOLD symbol will be flashing.

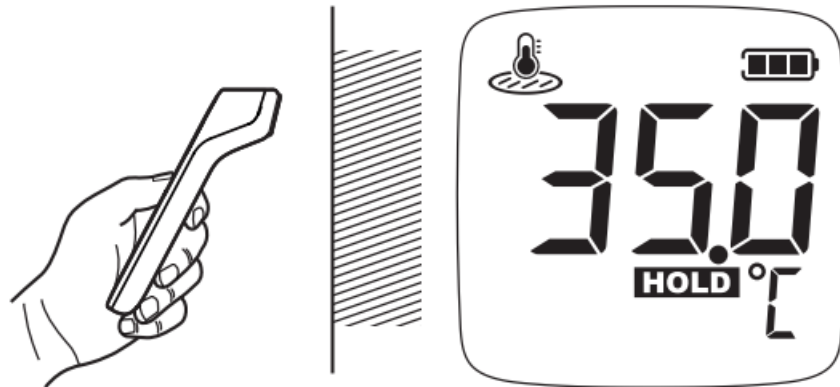


5. Release the button and read the result. If the reading is 0°C (32°F) and 100°C (212°F), the display will show the reading with green backlight.

**NOTE:**

- If the reading is 0.0°C, the display will show “Lo”. • If the reading is 100.1°C, the display will show “Hi”.

**CHANGING UNIT OF MEASUREMENT**

1. With the thermometer off, press and hold the MODE button for 1 second. The current unit of measurement will be flashing. The default setting is in °C.
2. Press the MODE button again to make a switch in the unit of measurement.

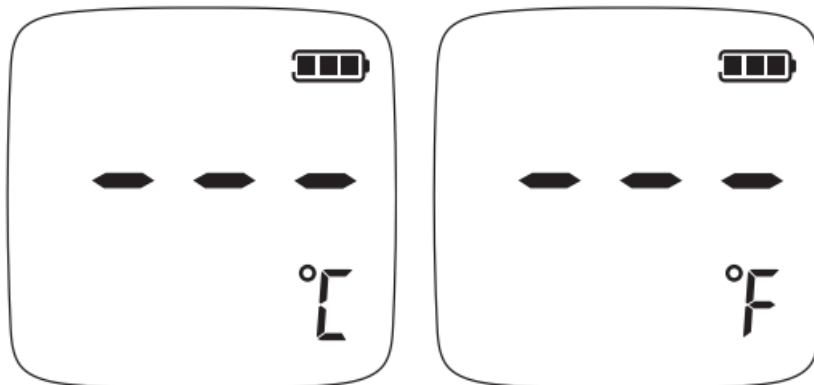

3. When finished, press the SCAN button to turn off the thermometer. The thermometer switches off automatically when left idle for 30 seconds.

**HINTS ON TAKING TEMPERATURES**

1. As with other thermometers, you may observe slight variations in consecutive measurements. It is recommended that you take 3 temperature readings and use the highest one for the following situations:
  - Infants are younger than 3 months old.
  - Children younger than 3 years old and who have a compromised immune system and the presence/absence of fever is critical.
  - When you are learning to use the thermometer.
2. Do not take a reading while the person is moving and/or talking. Wait 30 minutes after any of the following


situations before taking a measurement:

- When the forehead has been covered.
- After the person has been exercising, swimming, or taking a bath.
- When the person has been exposed to extreme temperature.

## RECALLING PAST READINGS

The TD-1242 stores 30 most recent readings.

1. Press and release the SCAN button to turn on the thermometer.
2. Press and hold the MEMORY button for 1 second to enter the memory mode indicated by a flashing “M” symbol. The most recent reading stored will be displayed.

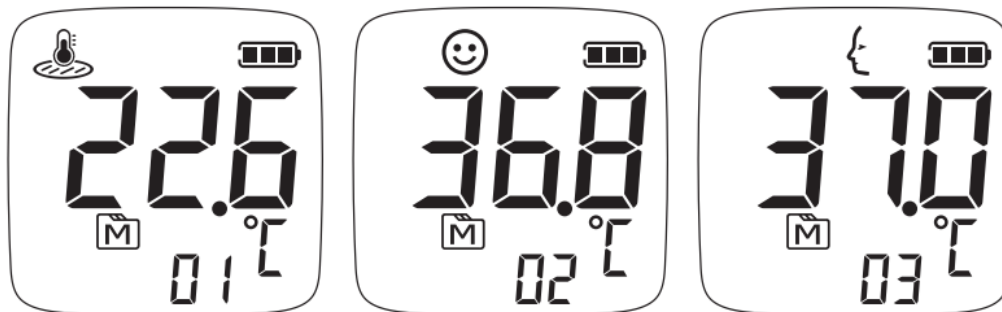

3. Press and release the MEMORY button to cycle through older readings.
4. When left idle for 30 seconds, the thermometer automatically switches off.

### NOTE:

When the memory is full, the oldest result is deleted as the new ones are added. While recalling previous readings, you may take a measurement by pressing the SCAN button.

## NORMAL BODY TEMPERATURE & FEVER

Body temperature can vary from one individual/person to the next. It also varies by location on the body and time of day. Fever indicates that the body temperature is higher than normal. This symptom may be caused by infection, overdressing, or immunization. Some people may not experience fever even when they are ill. These include, but are not limited to, infants younger than 3 months old, persons with compromised immune systems, persons taking antibiotics, steroids, or antipyretics (aspirin, ibuprofen, acetaminophen), or persons with certain chronic illnesses.

Body Site Normal Temperature Range	
Oral	0.6°C (1°F) or more above or below 37°C (98.6°F)
Rectal / Ear	0.3°C to 0.6°C (0.5°F to 1°F) higher than an oral temperature
Axillary (armpit)	0.3°C to 0.6°C (0.5°F to 1°F) lower than an oral temperature






Source: Body Temperature at WebMD; website: <http://firstaid.webmd.com/body-temperature> retrieved at 2010 Jan 7.

Please consult your physician if you are concerned about your body temperature readings.












## MAINTENANCE

- The TD-1242 has no user-serviceable internal parts except battery replacement.
- Store in a dry location free of dust and away from direct sunlight.
- Use a soft dry cloth to clean the plastic housing or a cloth dampened with a solution of water and mild detergent. Occasionally, 70% isopropanol solution may be used. Never submerge in liquid.
- The sensor window is recessed to assist in keeping it clean and free of debris. Inspect the lens and remove any debris. Smudges may be cleaned by gently wiping the window with a small foam-tipped swab (non-lining) moistened with 70% alcohol. Wait 10 minutes prior to taking temperatures.

## TROUBLESHOOTING

MESSAGE	WHAT IT MEANS	WHAT TO DO
	Appear when the ambient temperature is outside of the operating temperature range.	Only operate the thermometer in the ambient temperature range of 10°C to 40°C (50°F to 104°F).
	Measured temperature below the measurement range (below 32.0 °C).	Review instructions and repeat measurement. Make sure the distance from the forehead is not greater than 7cm (2"), and that the forehead is clear.
	Measured temperature above the measurement range (above 43.0 °C).	Review instructions and repeat measurement. Consult with a physician if the problem persists.
	Low or no power.	Replace with new batteries.
	Surface temperature measured outside of the range (0.0 to the procedure) re-start the measurement	Review the instructions and measurement range (0.0 to the procedure).

## SYMBOL INFORMATION

Symbol	Referent	Symbol	Referent
	Consult instructions for use		Type BF applied part
	Manufacturer		Temperature limit
	Serial number		Serial number
	Serial number	<b>IP22</b>	Resistant to liquid ingress
	CE mark		RoHS Compliance
	This device does not belong to household waste and must be returned to a collection point for recycling electric and electronic devices according to local laws. If it contains batteries, the batteries should be removed and disposed of in accordance with local regulations for a separate collection of spent batteries.		
	Authorized Representative in the European Community		

## SPECIFICATIONS

Model No.: TD-1242

Dimension & Weight: 155.46 (L) x 40.14 (W) x 39.45 (H) mm, 61.8g (without battery)

Power Source: 2 x 1.5V AAA alkaline batteries

Battery Life: With new batteries, approx. 3,000 measurements.

Displayed Temperature range

- Forehead: 32°C to 43°C (89.6°F to 109.4°F)
  - Surface: 0°C to 100°C (32°F to 212°F)
- Display Resolution: 0.1°C / 0.1°F
- Accuracy: Meet the accuracy requirement specified in ASTM E1965-98 and ISO 80601-2-56
- Forehead:  $\pm 0.2^{\circ}\text{C}$  ( $\pm 0.4^{\circ}\text{F}$ ) for the range of 35.0°C to 42.0°C (95°F to 107.6°F) /  $\pm 0.3^{\circ}\text{C}$  ( $\pm 0.5^{\circ}\text{F}$ ) for the range of  $<35.0^{\circ}\text{C}$  (95°F) or  $>42.0^{\circ}\text{C}$  (107.6°F)
  - Surface:  $\pm 1^{\circ}\text{C}$  ( $\pm 2^{\circ}\text{F}$ )
- Temperature Unit: °C (Default) or °F
- Operating Temperature range: 10°C to 40°C (50°F to 104°F)
- Operating Humidity: 30% to 85% relative humidity (non-condensing)
- Operating Atmosphere Pressure: 700hPa to 1060hPa Storage / Transportation Temperature range: -20°C to 60°C (-4°F to 140°F)
- Storage / Transportation Humidity: 30% to 85% relative humidity (non-condensing)
- Memory Capacity: 30 measurements
- Ingress Protection Rating: IP22
- The specifications may be changed without prior notice.

## REFERENCE STANDARDS

**Device Standard:**

Device Corresponds to the requirements of the standard for infrared thermometers ASTM E1965-98, EN ISO 80601-2-56:2017, EN 60601-1-2:2015, EN 60601-1:2006+A12:2014, EN 60601-1-6:2010

**Electromagnetic Compatibility:**

The device fulfills the stipulations of the standard EN 60601-1-2. The stipulations of EU-Directive 93/42/EEC for Medical Devices Class IIa have been fulfilled.

<b>Manufacturer's declaration-electromagnetic emissions</b>		
<b>The TD-1242</b> is intended for use in the electromagnetic environment (for home and professional healthcare) specified below. The customer or the user of the TD-1242 should assure that it is used in such an environment.		
<b>Emission test</b>	<b>Compliance</b>	<b>Electromagnetic environment-guidance (for home and professional healthcare environment)</b>
RF emissions CISPR 11	Group 1	The TD-1242 uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.  The TD-1242 is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
RF emissions CISPR 11	Class B	
Harmonic emissions IEC 61000-3-2	Not applicable	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Not applicable	

## Manufacturer's declaration-electromagnetic immunity

The TD-1242 is intended for use in the electromagnetic environment (for home and professional healthcare) specified below. The customer or the user of the TD-1242 should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment-guidance (for home and professional healthcare environment)
Electrostatic discharge(ESD) IEC 61000-4-2	Contact:±8 kV Air2 kV,±4 kV, ±8 kV,±15 kV	Contact:±8 kV Air±2 kV,±4 kV, ±8 kV,±15 kV	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%
Electrical fast transient/burst IEC 61000-4-4	+ 2kV for power supply lines + 1kV for input/output lines	Not applicable Not applicable	Mains power quality should be that of a typical home and professional healthcare environment.
Surge IEC 61000-4-5	+ 0.5kV, +1kV line(s) to line(s) + 0.5kV, +1 kV,+2kV line(s) to earth	Not applicable Not applicable	The mains power quality should be that of a typical home and professional healthcare environment.
Voltage Dips, short interruptions, and voltage variations on power supply input lines IEC 61000-4-11	Voltage dips: 0 % UT; 0,5 cycle 0 % UT; 1 cycle 70 % UT; 25/30 cycles Voltage interruptions: 0 % UT; 250/300 cycle	Voltage dips: Not applicable, Not applicable Not applicable  Voltage interruptions: Not applicable	The mains power quality should be that of a typical home and professional healthcare environment. If the user of the TD-1242 requires continued operation during power mains interruptions, it is recommended that the TD-1242 be powered from an uninterruptible power supply or a battery.
Power frequency (50, 60 Hz) magnetic field IEC 61000-4-8	30 A/m 50 Hz or 60 Hz	30 A/m 50 Hz and 60 Hz	The TD-1242 power frequency magnetic fields should be at levels characteristic of a typical location in a typical home healthcare environment.

**NOTE UT** is the a.c. mains voltage prior to application of the test level.

## Manufacturer's declaration-electromagnetic immunity

**The TD-1242** is intended for use in the electromagnetic environment (for home and professional healthcare) specified below. The customer or the user of the TD-1242 should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment-guidance (for home and professional healthcare environment)
Conducted RF IEC 61000-4-6R radiated RF IEC 61000-4-3	<p>3 Vrms:</p> <p>0,15 MHz — 80 MHz 6 Vrms:</p> <p>in ISM and amateur radio bands between 0,15 MHz and 80 MHz</p> <p>80 % AM at 1 kHz</p> <p>10 V/m</p> <p>80 MHz — 2,7 GHz 80 % AM at 1 kHz</p>	<p>Not applicable</p> <p>Not applicable</p> <p>10 V/m</p> <p>80 MHz — 2,7 GHz 80 % AM at 1 kHz</p>	<p>Portable and mobile RF communications equipment should be used no closer to any part of the TD-1242 including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance: <math>d = 1,2 \cdot \sqrt{P}</math></p> <p><math>d = 1,2 \cdot \sqrt{P}</math> 80MHz to 800 MHz <math>d = 2,3 \cdot \sqrt{P}</math> 800MHz to 2,7 GHz</p> <p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol: (V)</p>

**NOTE1** At 80 MHz and 800 MHz, the higher frequency range applies.

**NOTE2** These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

**The recommended separation distance between portable and mobile RF communications equipment and the TD-1242**

The TD-1242 is intended for use in an electromagnetic environment (for home and professional healthcare) in which radiated RF disturbances are controlled. The customer or the user of the TD-1242 can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the TD-1242 as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz $d = 1,2A1P$	80 MHz to 800 MHz $d = 1,2 \sqrt{P}$	800 MHz to 2,7 GHz $d = 2,34P$
0,01	N/A	0,12	0,23
0,1	N/A	0,38	0,73
1	N/A	1,2	2,3
10	N/A	3,8	7,3
100	N/A	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $p$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

**NOTE1** At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

**NOTE2** These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

**Manufacturer's declaration-electromagnetic immunity**

Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment

The TD-1242 is intended for use in the electromagnetic environment (for home and professional healthcare) specified below. The customer or the user of the TD-1242 should assure that it is used in such an environment.

Test frequency (MHz)	Bandy (MHz)	Service 4	Modulation type	Maximum power (W)	Distance (m)	IMMUNITY TEST LEVEL (V/m)	Compliance LEVEL (V/m) (for home and professional healthcare)
385	380 -390	TETRA 400	Pulse modulation b) 18 Hz	1,8	0,3	27	27
450	430 – 470	GMRS 460 FRS 460 5	FM c) ±5 kHz deviation 1 kHz sine	2	0,3	28	28
710	704 – 787	LTE Band 13, 17	Pulse modulation b) 217 Hz	0,2	0,3	9	9
745							
780							
810	800 – 960	GSM 800/1900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation b) 18 Hz	2	0,3	28	28
870							
930							
1 720	1 700-1 990	GSM 1800; CDMA 1900; GSM 1900: DECT: LTE Band 1, 3, 4, 25; UMTS	Pulse modulation b) 217 Hz	2	0,3	28	28
1 845							
1 970							
2 450	2 400 – 2 570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation b) 217 Hz	2	0,3	28	28
5 240	5 100 – 5 800	WLAN 802.11 a/n	Pulse modulation b) 217 Hz	0,2	0,3	9	9
5 500							
5 785							

NOTE If necessary to achieve the IMMUNITY TEST LEVEL, the distance between the transmitting antenna and the ME EQUIPMENT or ME SYSTEM may be reduced to 1 m. The 1 m test distance is permitted by IEC 61000-4-3.

- a) For some services, only the uplink frequencies are included.
- b) The carrier shall be modulated using a 50 % duty cycle square wave signal.
- c) As an alternative to FM modulation, 50 % pulse modulation at 18 Hz may be used because while it does not represent actual modulation, it would be the worst case.

## Documents / Resources



[TaiDoc TD-1242 Forehead Thermometer](#) [pdf] Instruction Manual  
TD-1242, Forehead Thermometer