


**Teleflex®**  
PB-45703-200  
Pressure  
Injectable  
Three Lumen  
PICC

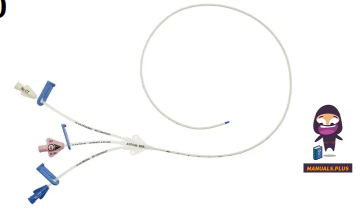

## Teleflex PB-45703-200 Pressure Injectable Three Lumen PICC Instructions


[Home](#) » [Teleflex](#) » Teleflex PB-45703-200 Pressure Injectable Three Lumen PICC Instructions 

### Contents

- [1 Teleflex PB-45703-200 Pressure Injectable Three Lumen PICC](#)
- [2 Product Description](#)
- [3 Instruction](#)
- [4 Features](#)
- [5 Specifications](#)
- [6 FAQs](#)
- [7 Documents / Resources](#)
  - [7.1 References](#)
- [8 Related Posts](#)

**Teleflex®**

**Teleflex PB-45703-200 Pressure Injectable Three Lumen PICC**

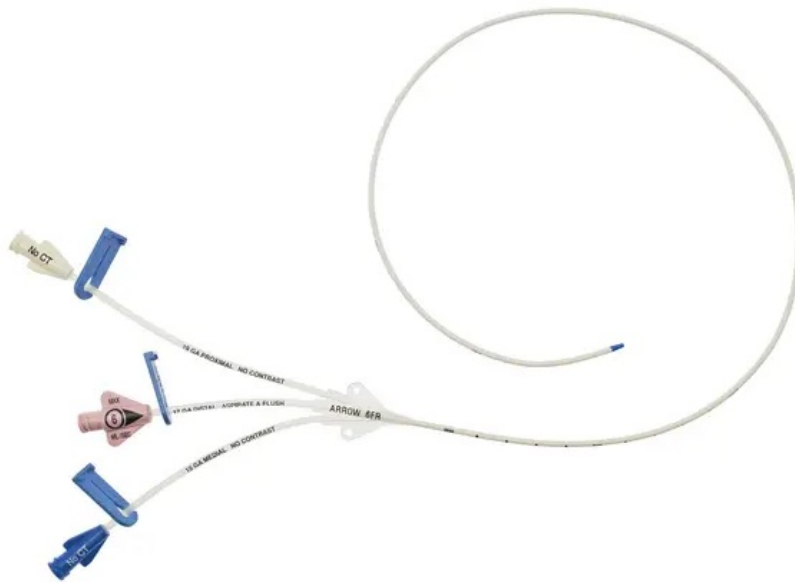

## Product Description


- 1: Three Lumen Catheter: 6 Fr. (2.14 mm OD) x 50 cm, Pressure Injectable, TPort Connector, Blue FlexTip®, Contamination Guard and Placement Wire
- 1: GlideThru™ Peel-Away Sheath: 6 Fr. x 2-3/4" (7 cm) Radiopaque over 6 Fr. Dilator
- 1: Spring-Wire Guide, Nitinol, Marked: .018" (0.46 mm) dia. x 17-3/4" (45 cm) (Straight Soft Tip on One End – Straight Stiff Tip on Other) with Arrow Advancer
- 1: Injection Needle: Eclipse™1 22 Ga. x 1-5/8" (4 cm)
- 1: Injection Needle: Eclipse™1 25 Ga. x 1" (2.54 cm)
- 1: Introducer Needle: Echogenic 21 Ga. x 2-3/4" (7 cm) TW
- 1: Filter Needle: 18 Ga. TW x 1-1/2" (3.81 cm) with Blunt Fill Tip
- 2: Syringe: 10 mL Luer-Lock
- 1: Syringe: 3 mL Luer-Lock
- 1: SecondSite™ Adjustable Hub: Fastener
- 1: SecondSite™ Adjustable Hub: Catheter Clamp
- 1: SharpsAway® II Locking Disposal Cup
- 1: SharpsAway® Disposal Cup
- 1: Catheter Trimmer
- 1: Towel: 24" x 36" (61 cm x 91 cm)
- 1: Drape: 60" x 76" (152 cm x 193 cm)
- 1: Drape: 36" x 41" (91 cm x 104 cm) with 3" x 5" (8 cm x 13 cm) fenestration
- 1: Towel
- 1: Safety Scalpel: #11
- 1: Patient ID Card
- 1: Sterile Procedure Sign
- 1: Patient Information Booklet
- 1: Chart Sticker
- 1: PICC Line Insertion Checklist
- 1: Paper Tape Measure
- 1: Tourniquet

- 5: Gauze Pad: 2" x 2" (5 cm x 5 cm)
- 10: Gauze Pad: 4" x 4" (10 cm x 10 cm)
- 1: Dressing: Tegaderm®2 I.V. Advanced 3-1/4" x 4-1/2" (8.5 cm x 11.5 cm)
- 1: Dressing: GRIP-LOK®3 Catheter Fixation Device
- 1: Surgical Apparel: Cap
- 1: Surgical Apparel: Impervious Gown
- 1: Dressing: Steri-Strip®2 1/2" x 4" (1.2 cm x 10 cm)
- 1: Surgical Apparel: Mask
- 1: Surgical Apparel: Mask with Shield
- 1: Transducer Cover: 4-12/16" x 95" (12 cm x 244 cm)
- 3: Valve: MicroCLAVE™4 Neutral Displacement Connector
- 1: HemoHopper® Fluid Receptacle
- 1A trademark of Becton, Dickinson and Company.
- 2A registered trademark of 3M Company.
- 3A registered trademark of TIDI.
- 4A trademark of ICU Medical, Inc.

All components are CE 2797 unless otherwise noted.

## Instruction

**Warning:** Read all package insert warnings, precautions, and instructions before use. Failure to do so may result in severe patient injury or death. [www.teleflex.com/IFU](http://www.teleflex.com/IFU) Not made with natural rubber latex. Fluid path components are non-pyrogenic. Contraindications: The Pressure Injectable PICC is contraindicated wherever there is the presence of device-related infections or the presence of thrombosis in the intended insertion vessel or catheter pathway. Clinical assessment of the patient must be completed to ensure no contraindications exist.

 Lumen	Priming Volume* (mL)	Gravity Flow Rate† (mL/hr)	Pump Flow Rate†† (mL/hr)	MAX Pressure Injection Flow Rate** (mL/sec)
Distal (17 Ga.)	0.62	1195	6410	6
Medial (19 Ga.)	0.42	297	2720	not rated
Proximal (19 Ga.)	0.45	297	2830	not rated

- Priming volumes are approximate and are done without accessories.
- Flow rate values are approximate and are determined using deionized water at 100 cm head height.
- Pump flow rates are determined at a maximum pump pressure of 10 psig and represent approximate flow capabilities.
- Pressure injection flow rates are determined at the injector pressure setting of 300 psi maximum using media of 11.8 centipoise viscosity, with 152 cm pressure tubing.

EU Authorized Representative and Importer:

Teleflex Medical IDA Business and Technology Park Dublin Road, Athlone Co. Westmeath, Ireland Contents: NO  
CT 6 EU-25063-HPMSB Pressure Injectable Three-Lumen PICC  
Arrow International LLC Subsidiary of Teleflex Incorporated 3015 Carrington Mill Blvd. Morrisville, NC 27560 USA

## Features



**LOT** Lot Number

YYYY-MM-DD

YYYY-MM-DD



(01)XXXXXXXXXXXXXX  
(17)YYMMDD  
(11)YYMMDD  
(10)Lot Number

**6** Fr. **3** Lumen **50** cm catheter length **.018** inch dia. spring-wire guide

## Specifications

- **Dimensions:** 11" (width) x 19" (length)
- **Model:** PB-45703-200
- **Dimensions:** 10 3/4" x 17 1/4"
- Product of xxx Packaged in xxx
- **Lumen:** 6
- **Length:** 50cm
- **Spring-wire guide diameter:** .018 inch
- Pressure Injectable Three-Lumen PICC

## FAQs

### Q: What are the contraindications for using the Pressure Injectable PICC?

A: The Pressure Injectable PICC is contraindicated wherever there is the presence of device-related infections or the presence of thrombosis in the intended insertion vessel or catheter pathway.

### Q: What is the priming volume for each lumen?

A: The priming volumes are approximately Distal – 0.62 mL, Medial – 0.42 mL, Proximal – 0.45 mL.

### Q: What are the flow rates for gravity and pump injections?

A: The gravity flow rates are Distal – 1195 mL/hr, Medial – 297 mL/hr, Proximal – 297 mL/hr. The pump flow rates are Distal – 6410 mL/hr, Medial – 2720 mL/hr, and Proximal – 2830 mL/hr.

## Documents / Resources



[Teleflex PB-45703-200 Pressure Injectable Three Lumen PICC \[pdf\] Instructions](#)  
PB-45703-200, PB-45703-200 Pressure Injectable Three Lumen PICC, Pressure Injectable Three Lumen PICC, Injectable Three Lumen PICC, Three Lumen PICC, PICC

## References

- [User Manual](#)

## **Manuals+. Privacy Policy**

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.