



Temtop M2000 2nd Generation Multi Functional Air Quality Detector User Manual

[Home](#) » [Temtop](#) » Temtop M2000 2nd Generation Multi Functional Air Quality Detector User Manual 



M2000 2nd Cogeneration Multi-functional Air Quality Detector User Manual

Contents

- [1 Factors Affecting Air Quality](#)
- [2 Important!](#)
- [3 Overview:](#)
- [4 Operation](#)
 - [4.1 View or Set PM2.5/CO²/HCHO](#)
 - [4.2 View all info](#)
- [5 History](#)
 - [5.1 Set](#)
- [6 Multipoint Detection](#)
- [7 OFF](#)
- [8 Specifications](#)
- [9 FAQ:](#)
- [10 What's Included](#)
- [11 Warranty](#)
- [12 Documents / Resources](#)
- [13 Related Posts](#)

Factors Affecting Air Quality



PM2.5 (Particulate Matter 2.5) refers to fine particles with a diameter of 2.5 micrometers or less. Due to its tiny size, PM2.5 can be absorbed into the bloodstream and the lungs, so that long-term exposure to the high concentration of PM2.5 environment may cause eye and nose irritation, cough, asthma, emphysema, lung disease, heart attacks, cancer and etc.



PM10 (Particulate Matter 10) refers to particulates with a diameter of 10 micrometers or less. Due to the larger size, it's inhalable but penetrates no further than bronchi as larger particles can be filtered out by cilia and mucus of the nose and throat. It normally considered less harmful to health than PM2.5.



Formaldehyde (HCHO) is a colorless and strong-smelling gas with the formula CH_2O , which has been classified by IARC as Group 1 carcinogen. Long-term exposure to just low doses could cause chronic respiratory diseases, nasopharyngeal carcinoma, colon cancer, brain tumors, nuclear gene mutation and etc.




TVOC (Total Volatile Organic Compounds) refers to various common ones including benzene, toluene, styrene, formaldehyde and etc. Due to their volatility as well as toxicity, irritability, and carcinogenicity, long-term exposure to TVOCs can cause damage to the skin, liver, kidneys, central nervous system and etc.



CO_2 (Carbon Dioxide) refers to a colorless and odorless gas that is usually derived from the breath of humans and animals. High CO_2 concentration means that fresh air or ventilation is required, otherwise, it may cause problems such as drowsiness, dizziness, loss of attention, and cognitive impairment.

Important!

- * Do not place the detector in heavily polluted environments (concentration of HCHO > 1.0mg/m or particle > 500g/m) for a long time; or it may cause damages to the sensor.
- * Do not cover the air inlet/outlet during detection; or let fluff or hair enter the detector.
- * Do not make contact with organic solvents, such as glue/adhesives/paint/alcohol, etc.

- * Do not use detectors in humid places or environments with a strong odor to maintain accuracy.
- * Do not use in environments containing gases listed in FAQ 6 to avoid influences on HCHO sensor.
- * If battery level shows , please charge the detector promptly to avoid effects during use (also chargeable when turned off).

Overview:



1. Buzzer Status
2. Measuring Status
3. Display
4. Menu Button
5. Increase/Up
6. USB Port
7. Date & Time
8. Battery Level
9. Back Button
10. Power/OK Button
11. Decrease/Down/Switch (Start/Pause) Button

Operation

warning!





- First use or unused for a long time: please put it outside over 6 hours for calibration.
- Indoor use: keep the room/area airtight for 10 minutes to obtain more accurate results.
- When calibrating the CO² and formaldehyde sensors, please adjust the detector to the calibration interface and place it outdoors in a cool and ventilated environment for S minutes.


Detection results will be much more accurate.

1. ON

Press and hold the power button  for 2 seconds to turn on the detector

2. Detection

Press  to enter the main menu interface (see the figure below), then press  or  to locate the option to view or set and press  to confirm.

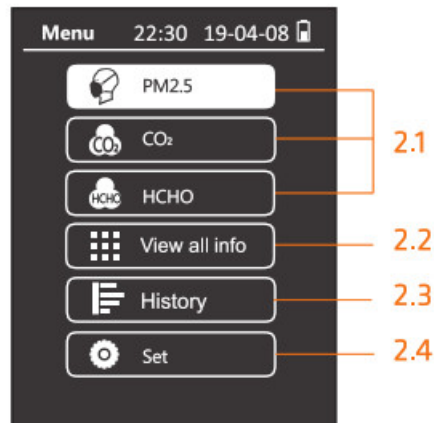

2.1 View or set particles/CO₂/HCHO



2.2 View all the information


2.3 Check data records

2.4 Set date, time, alarm value, help document, reset to default, and language.

Note: It takes about 3 minutes for the CO₂ sensor to warm up and then enter detection status.

View or Set PM2.5/CO₂/HCHO

In each interface, press  to display more functions. Take CO₂ interface, for example, press  button, you may see the following function options:

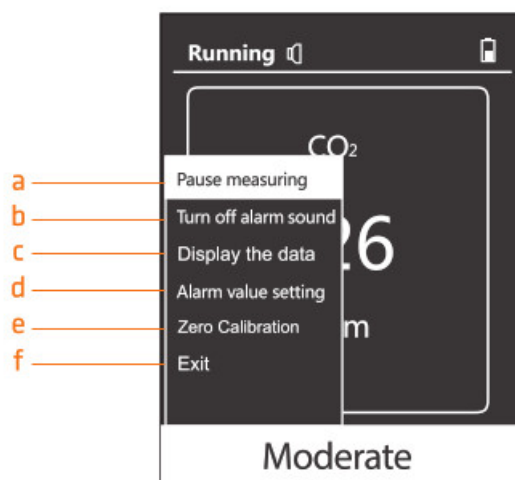





a. Pause measuring: Pause or restart detecting PM2.5.

b. Turn on/ off alarm sound: Mute/ Unmute the buzzer.

c. Display the curve: Display (or not) the PM2.5 concentration curve.

d. Alarm value setting: Set a high alarm limit.

Operation: Press  or  the button to adjust the value and press  to switch digits. Then Press Save and [to save the setting and exit the interface, or press Exit and  to exit without saving the setting (See the figure

below).



e. Zero calibration: Calibrate the sensor to zero (not available for PM2.5). Take the CO² interface below for example:




f. Exit: Exit current interface.

View all info

The **View all info** interface displays all the detected data including the concentration of PM2.5, PM10, CO2, HCHO, number of particles, temperature, and humidity.

Operation: Press  to switch between C°and °F (See the figures below).

Press  to pause or detect; press  to back to the main menu interface.

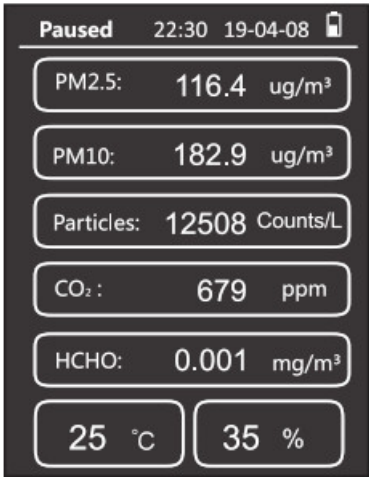




History


The **History** interface includes **Storage interval** and **Data export** functions (See the figure below).

Operation: Press  or  or switch between **Storage interval** and **Data export**, then press  to enter the corresponding interface.




a. Storage interval: Press  to switch between digits, **Save**, and **Exit**. When you select a digit, press A or .” to adjust the value to your desired storage interval among 1, 5, 10, 30 and 60 minutes, then locate the option to

Save and press  to save the setting and exit the interface; or locate the option to **Exit** and press  to exit the interface without saving the setting.

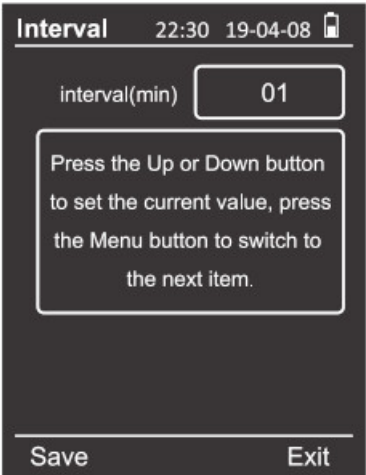

b. Data export: In this interface, you will see the following tips.

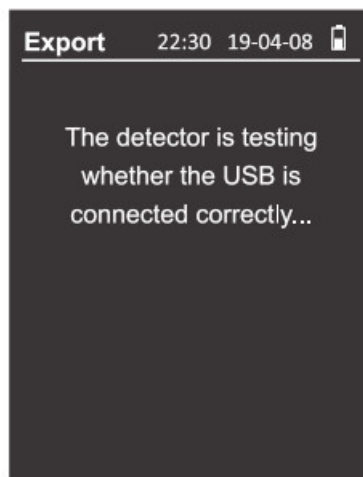


If connected to the computer successfully by the USB cable, the detector will pop up a tip **USB connection successful**; If not, it will remind you of the failure (See the figures below).



After connecting successfully, the detector will generate i **n the computer** a removable storage device **Temtop**, which contains a folder named History. The history folder includes a CSV format file listing the date and time PM2.5, PM10, CO2, and HCHO concentration (see the figure). Please save it to your computer for viewing.




Date	PM2.5	PM10	co	HOHO
2019/10/28 15:09	6	10	2038	0.081
2019/10/28 15:13	7	11	1795	0.071
2019/10/28 15:21	8	14	1914	0.059

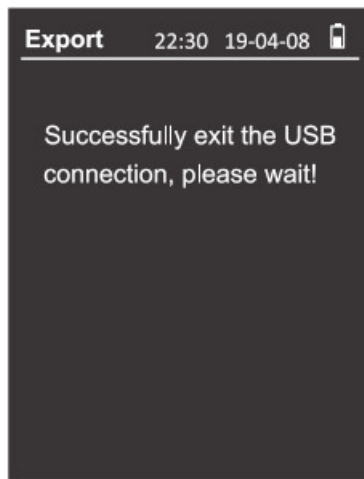
After the data is copied and viewed, please press  to exit and restart the detector (See the figure below).



Set



The Set interface displays 5 options below.

Operation: Press  or  to select the desired option; press  to enter the interface.

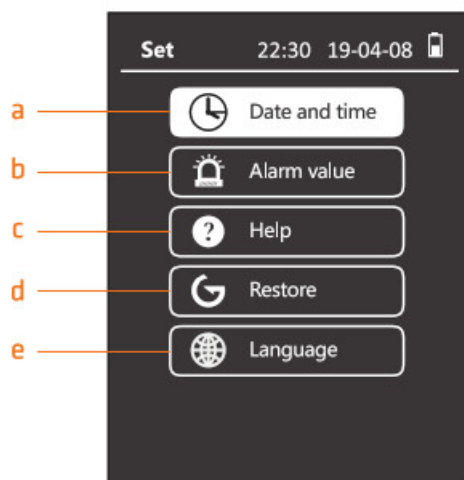

a. Date and time: Allows customized setting of year, month, date, and time (See the figure below).

Operation: Press  or  to adjust time and press  to switch to the next digit. Then press  to switch to **Save** or **Exit**. Press  to finish the settings and exit the interface.

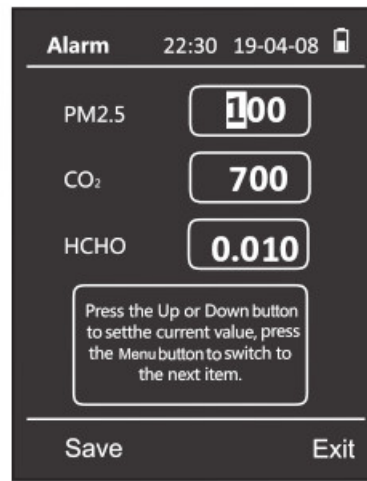
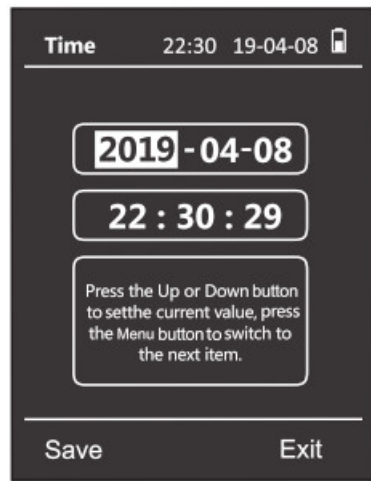


b. Alarm value: Set a high alarm limit for PM2.5, CO₂, or HCHO concentration (See the figure below).

Operation: Press or to set a high alarm limit for PM2.5, CO₂, or HCHO concentration and press to switch to the next digit. Then press to switch to **Save** or **Exit**. Press to finish the settings and exit the interface.

c. Help: View the help information for using the detector (See the figure below).

Operation: Press or to view the information that helps you use the detector; press to back to Set interface.

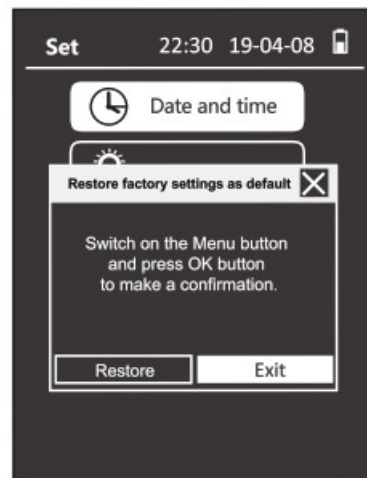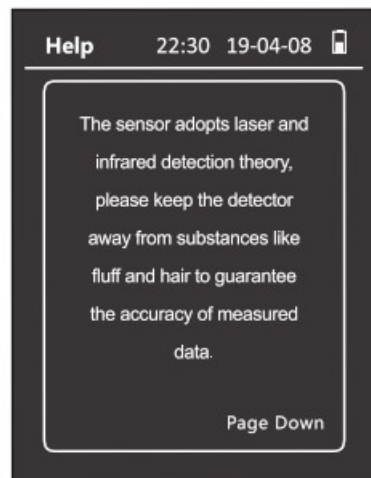


d. Restore: Reset to the default parameters (See the figure below).

Operation: Press to switch to **Restore** or **Exit**. Press to confirm the settings and exit the interface. If reset, all the customized settings will automatically turn to the default.

e. Language: Set Chinese or English as a displayed language (See the figure below).


Operation: Press to switch between Chinese and English, press to confirm; then press again to switch to **Save** or **Exit**; press to finish the settings and exit.

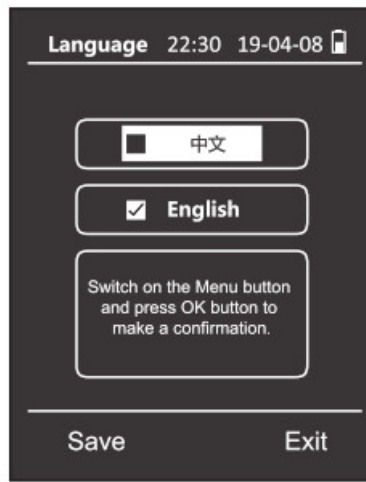

Multipoint Detection

Repeat **(2) Detection** at multiple points in the targeted area to get a more comprehensive understanding of your air quality.

OFF

The device will turn off automatically after 1 hour without any activity, you can also press and hold  for 2 seconds to turn off it manually.

Note: The auto-off function is invalid in the Histogram interface.

Specifications

Model	M2000 2nd Generation
Dimensions	223.5×73.5×37.5mm / 8.8×2.8×1.4in.
Battery capacity	3000mAh
Battery life	6-8h
Input	DC5V; 1A
Display	TFT color screen
Operation environment	Temperature range: 0-50°C (32-122°F) humidity range: 0-90% RH Atmospheric pressure condition: late
PM2.5	Sensor: Laser PM sensor Measuring range: 0-999 $\mu\text{g}/\text{m}^3$ Resolution: 0.1 $\mu\text{g}/\text{m}^3$ Accuracy: $\pm 10 \mu\text{g}/\text{m}^3$ (0-100 $\mu\text{g}/\text{m}^3$) $\pm 10\%$ (100-500 $\mu\text{g}/\text{m}^3$)
PM10	Sensor: Laser PM sensor Measuring range: 0-999 $\mu\text{g}/\text{m}^3$ Resolution: 0.1 $\mu\text{g}/\text{m}^3$ Accuracy: $\pm 15 \mu\text{g}/\text{m}^3$ (0-100 $\mu\text{g}/\text{m}^3$) $\pm 15\%$ (100-500 $\mu\text{g}/\text{m}^3$)
Carbon dioxide (CO2)	Sensor: Non-Dispersive Infrared (NOIR) CO ₂ sensor Measuring range: 0-5000 ppm Resolution: 1 ppm Accuracy: $\pm(50 \text{ ppm} + 5\% \text{ reading})$
HCHO	Optimum measurement range: 0-2 mg/m^3 Measurement limits: 5 mg/m^3 Resolution: 0.001 mg/m^3 Accuracy: $\pm 0.03 \text{ mg}/\text{m}^3$ (0-0.3 mg/m^3) $\pm 10\%$ (0.3-1 mg/m^3)

FAQ:

Q: Why is the data reading very high/over-range after the detector is turned on?

A: As being packed in ink printed package box over time may interfere with the sensor due to the remaining organic volatile residue inside the package. Therefore, after unpacking, please put the detector in a ventilated place to help accelerate its data recovery.

Q: Why is data reading unstable?

A: As airflow in the environment is changing, the distribution of organic matter concentration may be uneven. Temp recommends trying again in low airflow areas.

Q: Why is the test result abnormal or below normal?

A:

1. Please check whether the air inlet or outlet has been covered or fluid is in.
2. Gently shake the detector during detection to increase the interaction with the surrounding air.
3. The sensor may be not recovered. Please place the detector outdoors for ventilation.

Q: Can the calibration be accelerated if the detector is facing the outlet of the air conditioner/fan?

A: No. The temperature difference or airflow speed at the air conditioner/fan outlet is relatively high, which may cause condensation or temperature changes on the sensor, affecting its detection performance. Please put the detector outdoors in a cool ventilated place.

Q: Why is the PM2.5 reading constantly changing?

A: As PM2.5 concentration in the environment is changing all the time not only due to environmental factors like changes in airflow, humidity, wind direction and etc. but also due to common pollutant sources like smoking, cooking; exhaust emissions from vehicles, smoke from burning coal/chimneys/furnaces and etc. All these may influence the PM2.5 concentrations and give differences in the readings.

Q: Why is the HCHO reading inaccurate or overestimated at some points?

A: As Temtop uses a high-precision electrochemical HCHO sensor, its electrochemical reaction characteristics could also respond to other gases besides formaldehyde. This table lists the most common gases that interfere with the relative sensitivities of the HCHO sensor:

Interference Gas	Relative Sensitivity (%)
Carbon monoxide (CO)	1
Hydrogen (H ₂)	0.1
Ethyl alcohol	50
Phenols	7
Sulphur dioxide(SO ₂)	12
Ammonia (NH ₃)	0

Q: Which reference standards have been used to indicate the pollution levels?

A: Reference Standards for Particles and CO₂ are shown below.

Status	Good	Moderate	Unhealthy f or Sensitive G roups	Unhealthy	Very Unhealthy	Hazardous
Pollutant						
PM2.5 ($\mu\text{g}/\text{m}^3$)	≤ 12	12.1~35.4	35.5~55.4	55.5~150.4	150.5~250.4	≥ 250.5
PM10 ($\mu\text{g}/\text{m}^3$)	≤ 54	54.1~154	154.1~255	255.1~354	354.1~424	≥ 425
CO2 (PPm)	≤ 700	701~1000	1001~1500	1501~2500	2501~5000	≥ 5001

Reference Standard for HCHO is shown below.

Status	Healthy	Un Healthy
Pollutant		
HCHO (mg/m^3)	≤ 0.1	> 0.1

What's Included

Detector x 1
 USB Cable x 1
 User Manual x 1

Warranty

Temp warrants the included item for 1 year from the date of original purchase. The item can be exchanged or returned within 30 days if the defect is not caused by artificial damage.

Item	Warranty Period
Detector	1 year
Accessories	N/A

Before returning or sending for repair, please check if the following items are ready:

	Detector & Access ories	Complete Package	Proof of Purchase*	Gift (if any)
Return	√	√	√	√
Exchange	√	√	√	
Repair	√		√	

Including invoice, order number, etc.

Temp warranty does NOT include:

- Malfunction or damages caused by artificial damage or modification
- Other deliberate damages.
- Damages caused by force majeure events.



Elitech Technology, Inc.

2528 Qume Dr, Ste 2

San Jose, CA 95131 USA

Tel: +1408-898-2866

Sales: sales@temtopus.com

Website: www.temtopus.com

Elitech (UK) Limited

Unit 13 Greenwich Business Park,

53 Norman Road, London, SE10 9QF

Tel: +44 (0) 208-858-1888

Support: service@elitech.uk.com

Website: www.elitecheu.com

Elitech Brazil Ltda

R.Dona Rosalina,90 – Lgara, Canoas – RS 92410-695,Brazil

Tel: +(55)51-3939-8634


Sales: brasil@e-elitech.com

Website: www.elitechbrasil.com.br



V1.2

Documents / Resources

 <small>M2000 2nd Generation Multi-Functional Air Quality Detector User Manual</small>	Temtop M2000 2nd Generation Multi Functional Air Quality Detector [pdf] User Manual M2000, 2nd Generation Multi Functional Air Quality Detector, M2000 2nd Generation Multi Functional Air Quality Detector, Air Quality Detector, Quality Detector, Detector
--	--