

Fast Read Digital Clinical Thermometer KD-1470 \ KD-1471 Instruction Manual

[Home](#) » [Thermometer](#) » Fast Read Digital Clinical Thermometer KD-1470 \ KD-1471 Instruction Manual 

Fast Read Digital Clinical Thermometer KD-1470 \ KD-1471



INSTRUCTIONS FOR USE

Please Read Carefully before using the device


FEATURES

1. Fast oral and rectal temperature measurement in around 10 seconds with proper use.
2. Memory displays for the last temperature taken.
3. Very sensitive unit, best for quick oral or rectal measurement.
4. Easy to read digital LCD (liquid crystal display).
5. Compact, accurate and durable LSI (large scale integration) unit.
6. Temperature can be taken orally or rectally.
7. If the thermometer is inadvertently left on after temperature stabilization , it will automatically shut off in about 3 minutes.
8. Small , light weight unit. Universal use for the whole family. especially ideal for children.
9. ABS resin body presents no hazard compared to broken mercury /glass thermometers.
10. Low battery indicator : when the symbol " D "appears , the battery needs to be replaced .
11. This unit is waterproof.

PARTS DESCRIPTION

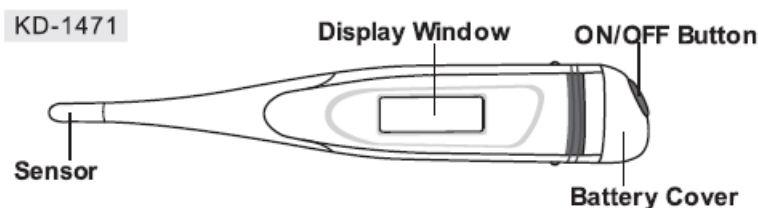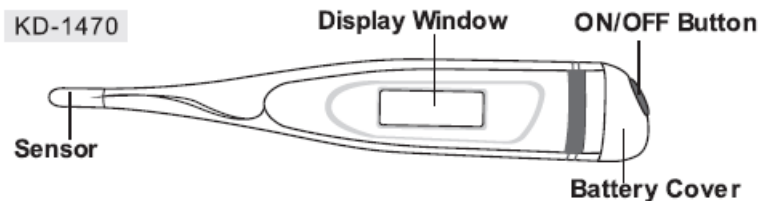

SPECIFICATIONS

Range :	32.0~43.9°C(90~109.9°F) Below 32.0°C(90.0°F) displays L°C(°F) Above 43.9°C(109.9°F) displays H°C(°F)
Resolution :	0.1 °C(°F)
Accuracy :	±0.1°C (34.0°C to 42.0°C); ±0.2°C(other range) ±0.2°F(93.2°F to 107.6°F); ± 0.4°F(other range)
Display :	Liquid crystal display 3 1/2 digits
Battery : (included)	Micro Alkaline battery 192, LR41 1.55V
Power Consumption :	0.15 milliwatts in measurement mode
Battery Life:	More than 200 hours of continuous operation
Dimensions :	Approx. 128mm x 20mm x 12mm
Weight :	Approx. 14.8grams including battery
Beeper :	Approx. 8 seconds sound signal when peak temperature reached
Memory :	Built-in memory enabling display of previously measured value
Working Conditions :	Temperature: 10 ~ 40°C(50 ~ 104°F) Relative Humidity: 15 ~ 95% non condensing
Storage Conditions:	Temperature: -20~ 60°C(-40 ~ 140°F) Relative Humidity: 15 ~ 95% non condensing
Guarantee of Quality :	Certification ISO 13485 Comply with ASTM-E1112, EN12470-3, EN60601-1
Product Classification :	Type BF  equipment

PRECAUTION

1. For best results, do not use the fast read thermometer for axillary (underarm) measurement. Only use it for taking oral and rectal temperatures.
2. Do not boil the probe . Instead , clean the unit by wiping it with a dry cloth and disinfect the probe with isopropyl(rubbing) alcohol .
3. Do not drop the thermometer or expose to heavy shock . The unit is not shock proof.
4. Do not bend or bite the probe .
5. Do not store the unit in direct sunlight, or at a high temperature, or in high humidity or dust. Performance may be degraded.
6. Stop using the thermometer if it operates erratically or if display malfunctions .
7. Keep out of the reach of unsupervised children .
8. Clean the thermometer probe before storing .
9. Do not attempt to disassemble the unit except to replace the battery .
10. If the thermometer has been stored at below-freezing temperatures, allow the thermometer to warm naturally to room temperature before using .
11. Performance of the device may be degraded if operated or stored outside stated temperatures and humidity

ranges or the patient's temperature is below the ambient (room) temperature.

BATTERY REPLACEMENT


1. When the symbol " **BATTERY** " appears , the battery needs to be replaced .
2. Pull the battery cover off in the direction shown.
3. Using a pointed object such as a toothpick or insulated probe to pry loose the old battery. Avoid using any sharp metal object in this operation.
4. Clean battery contacts and also those of the device prior to battery re-installation.
5. Place a new 1.55 VDC button size battery type 192, LR 41 or equivalent in the chamber with the negative (-) side up and the positive (+) side down .
6. Replace and fasten the battery cover securely .



Warning : Discard old battery carefully , out of reach of young children . Swallowing the battery may be fatal . If the battery is swallowed , contact a hospital immediately to have it removed . Do not dispose of the battery in a fire . It may explode .

HOW TO USE

1. Disinfect the probe with isopropyl(rubbing) alcohol before using
2. Depress the ON/OFF button. The display will read



3. Release the power switch and the display will show L°C(L°F)with °C(°F)flashing.
4. Place the probe in the appropriate position (oral, axillary or rectal).

4. Once the degree sign °C(°F) on the display has stopped flashing, the correct temperature is indicated. The temperature reading will not change after the °C(°F) stops flashing.

5. The unit will automatically turn off in 3 minutes (approx.). However, to prolong battery life, it is best to turn the thermometer off by pressing the ON/OFF button once the temperature has been noted.

Special Features:

Normal Temperature Alarm: An alarm will sound when the peak temperature has registered and is ready-to-read. The “Normal Temperature” alarm (four quick beeps followed by a pause) will sound repeatedly for approximately 8 seconds.

Last-Temperature Memory Recall: When the ON/OFF button is depressed to activate the thermometer, hold down for approximately 5 seconds. The display of 188.8 will change to show the last measured temperature. This reading is displayed as long as the button is held down. When the button is released, the thermometer will be in “ready-to-measure” mode and the recalled temperature will be erased.

For Models with Fever Alarm : If the temperature registers higher than 37.5°C(99.5°F), the fever alarm (a quick beeping sound which occurs continuously for about 8 seconds) will sound when the peak temperature has registered. Also, the result will keep flashing until the thermometer is turned off.

To change the scale from Fahrenheit (°F) to Centigrade (“C”): After turning the thermometer on, immediately press the ON/OFF button again and release. The °F changes to a °C. Once the display shows an L with a flashing °F or °C, the device is ready to record and display a temperature. Follow the same directions to switch back from Centigrade to Fahrenheit.

NOTE : Always disinfect the thermometer before using.

NOTE : In Step 2, if the room temperature is greater than 32.0°C (90.0°F), it will be displayed rather than L°C(or L°F).


NOTE : In Step 3, you may put a sanitary plastic probe shield on the sensor tip to help prevent cross-infection and contamination. Use of the probe cover may result in a 0.1 °C (0.2°F) difference from actual temperature. Dispose of any used probe shield and store the unit in a safe place.

RELIABLE METHODS TO MEASURE TEMPERATURE

THE TAKING OF BODY TEMPERATURES: Change in body temperature is one of the most important indicators of illness. It is important that accurate temperatures be taken. Even though the digital thermometer is used in similar manner to the glass thermometer, it is important that the simple instructions for use of this thermometer be followed closely and that the person taking the temperature understands body temperature.

BODY TEMPERATURE: A person’s body temperature will usually be several tenths to one full degree lower in the morning than it is in the late afternoon. Therefore, if your temperature is 36.6°C(97.9°F) in the morning, it could be 36.9°C(98.4°F) or more in the late afternoon and still be normal. To determine what your normal body temperature is you should take your temperature both in the early morning and in the late afternoon over several days. Children have the same normal temperature range as do adults. A fever for both children and adults is typically defined as a temperature over 37.5°C(99.5°F) (oral reading). Exercise, excessive clothing, hot bath, hot weather, warm food and drink can cause mild elevations of up to 38°C (100.4°F) to 38.4°C(101.1 °F) in oral temperature. If you suspect one of these to be the cause of an elevated reading, eliminate the possible cause and retake the temperature in a half hour.

ORAL USE

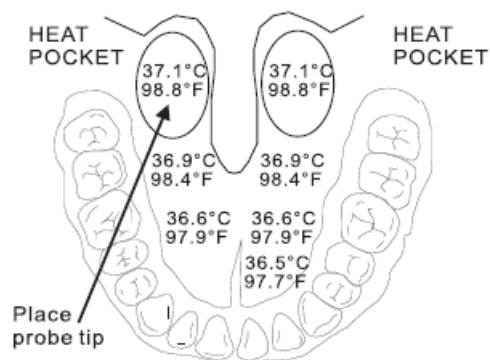

Place the probe well under the patient's tongue. Instruct the patient to keep their mouth closed while the thermometer is reading. A normal temperature by this method is usually considered between 36.0°C to 37.5°C (96.8°F to 99.5°F).

RECTAL USE

If rectal temperature is recommended by your doctor, you may use a probe shield. Insert thermometer into the probe shield. Lubricate the probe cover with a water soluble jelly for easier insertion. Do not use petroleum jelly. Insert tip of probe no more than 1/2 inch into rectum. STOP if you meet any resistance. The sensing unit is on the very tip of the probe and there is no need to insert the probe deep into the rectum. In general, the rectal temperature is around 0.5°C to 1.0°C (1.0 to 2.0°F) higher than oral temperature.

AXILLARY USE

Wipe armpit with a dry towel. Place probe in the patient's armpit and keep the patient's arm pressed firmly against the body. In general, the axillary temperature is around 0.5°C to 1.0°C (1.0 to 2.0°F) lower than oral temperature. Note that in order to achieve better axillary temperature measurement result a minimum measuring time of 2-3 minutes is recommended regardless of the beep sound.

NOTE : Children should be attended by an adult during the entire temperature recording process. After use, the digital thermometer should be stored in a safe place, out of reach of young children. If you compare temperatures between two thermometers, it is possible to have two different readings even if both thermometers are within their accuracy tolerances. Differences in how you take each reading and the thermometer's tolerance range can account for nearly 0.1°C (0.2°F) variability.

CLEANING INSTRUCTIONS

To clean the thermometer, wash the tip with a solution of mild detergent and cool water. Disinfect the thermometer by wiping the sensor and lower stem with a cloth dipped in a household antiseptic solution such as rubbing alcohol.

This thermometer may also be sanitized in a dishwasher. To wash in a dishwasher, please set the dishwasher in the "normal wash mode" with the "heated dry mode" turned to the off position. When washing the thermometer, please position it with tip down and main body up. The thermometer is guaranteed for up to 10 times of dishwasher cycle washing in the "normal wash mode."

LIMITED WARRANTY

This thermometer is guaranteed for one year from the date of purchase against manufacturer's defect under normal, household use. Following the directions closely will ensure years of dependable operation.

If the thermometer does not function properly, first check the battery (see battery replacement instructions). Replace it if necessary.

If the thermometer does not function properly, please write 180 INNOVATIONS at 11100 West 8th Ave, Lakewood, CO 80215 or call customer service at 1-877-299-6700. Our representative will provide further instruction on how to correct the trouble or will ask you to return it for repair or replacement.

FCC STATEMENT

NOTE: POTENTIAL FOR RADIO/TELEVISION INTERFERENCE (for U.S.A. Only)

This product has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. The product generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If the product does cause harmful interference to radio or television reception, which can be determined by turning the product on and off, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the product and the receiver.
- Connect the product into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

POTENTIAL FOR RADIO/TELEVISION INTERFERENCE (for Canada Only)

This digital apparatus does not exceed the Class B limits for radio noise emissions from digital apparatus as set out in the interference-causing equipment standard entitled "Digital Apparatus", ICES-003 of the Canadian Department of Communications. Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

[**KD-1470-and-KD-1471-Fast-Read-Digital-Clinical-Thermometer-User-Manual**](#)

Download

Questions about your Manual ? Post in the comments!