



TROTEC BM22 Moisture Measuring Device User Manual

[Home](#) » [TROTEC](#) » TROTEC BM22 Moisture Measuring Device User Manual 

Contents

- [1 TROTEC BM22 Moisture Measuring Device](#)
- [2 Safety](#)
- [3 Information about the device](#)
- [4 Display](#)
- [5 Technical data](#)
- [6 Transport and storage](#)
- [7 Operation](#)
- [8 Maintenance and repair](#)
- [9 Errors and faults](#)
- [10 Disposal](#)
- [11 Documents / Resources](#)
- [12 Related Posts](#)

TROTEC

TROTEC BM22 Moisture Measuring Device



Safety

Read this manual carefully before starting or using the device. Always store the manual in the immediate vicinity of the device or its site of use.

Warning

Read all safety warnings and all instructions. Failure to follow the warnings and instructions may result in electric shock, fire and/or serious injury. Save all warnings and instructions for future reference.

- Do not use the device in potentially explosive rooms or areas and do not install it there.
- Do not use the device in aggressive atmosphere.
- Do not immerse the device in water. Do not allow liquids to penetrate into the device.
- The device may only be used in dry surroundings and must not be used in the rain or at a relative humidity exceeding the operating conditions.
- Protect the device from permanent direct sunlight.
- Do not expose the device to strong vibrations.
- Do not remove any safety signs, stickers or labels from the device. Keep all safety signs, stickers and labels in legible condition.
- Do not open the device.
- Never charge batteries that cannot be recharged.
- Different types of batteries and new and used batteries must not be used together.
- Insert the batteries into the battery compartment according to the correct polarity.

- Remove discharged batteries from the device. Batteries contain materials hazardous to the environment. Dispose of the batteries according to the national regulations.
- Remove the batteries from the device if you will not be using the device for a longer period of time.
- Never short-circuit the supply terminal in the battery compartment!
- Do not swallow batteries! If a battery is swallowed, it can cause severe internal burns within 2 hours! These burns can lead to death!
- If you think batteries might have been swallowed or otherwise entered the body, seek medical attention immediately!
- Keep new and used batteries and an open battery compartment away from children.
- Observe the storage and operating conditions (see Technical data).

Intended use

Only use the device for moisture measurements of wood and building materials within the measuring range specified in the technical data.

To use the device for its intended use, only use accessories and spare parts which have been approved by Trotec.

Foreseeable misuse

Do not use the device in potentially explosive atmospheres, for measurements in liquids or at live parts.

Any unauthorized changes, modifications or alterations to the device are forbidden.

Personnel qualifications

People who use this device must:

have read and understood the operating manual, especially the Safety chapter.

Residual risks

- Warning of electrical voltage
- There is a risk of a short-circuit due to liquids penetrating the housing!
- Do not immerse the device and the accessories in water. Make sure that no water or other liquids can enter the housing.
- Warning of electrical voltage
- Work on the electrical components must only be carried out by an authorised specialist company!
- Risk of suffocation!
- Do not leave the packaging lying around. Children may use it as a dangerous toy.
- The device is not a toy and does not belong in the hands of children.
- Dangers can occur at the device when it is used by untrained people in an unprofessional or improper way! Observe the personnel qualifications!
- When handling the device there is a risk of injury due to the exposed measuring tips.
- Always put on the protective cap when not in use.
- Keep a sufficient distance from heat sources.
- **Note**
- Exclusively use the original measuring tips included in the scope of delivery. Other measuring tips might bend or damage the holder at the measuring device.
- Never force the measuring device into the material to be measured or yank it out. Applying force can lead to bending or breaking of the measuring tips or to the destruction of the housing.


- To prevent damage to the device, do not expose it to extreme temperatures, extreme humidity or moisture.
- Do not use abrasive cleaners or solvents to clean the device.

Information about the device

Device description


By use of the moisture measuring device BM22, the humidity level of wood and building material can be determined. Additionally, the ambient temperature can be measured in °C or °F.

Three-colour LED display for a quick assessment of the humidity level.

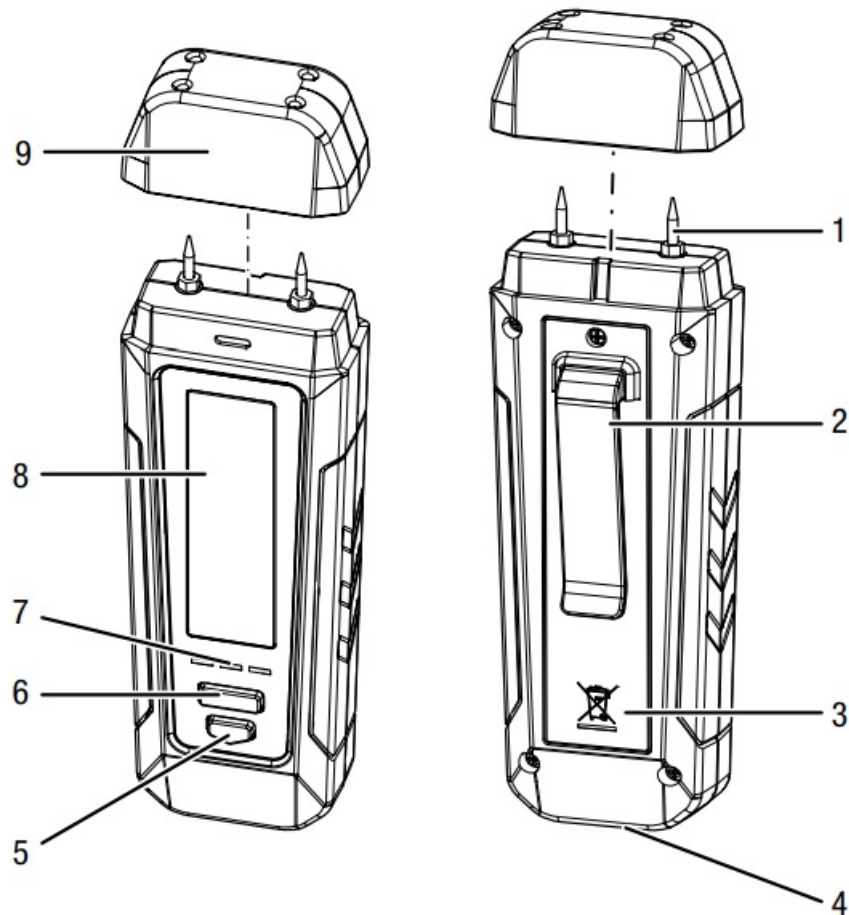

No.	Designation
1	Measuring tips
2	Transport clip
3	Battery compartment with cover
4	LED illumination
5	Lamp button
6	SET/ON button
7	LED display (green / yellow / red)
8	Display
9	Protective cap

Display

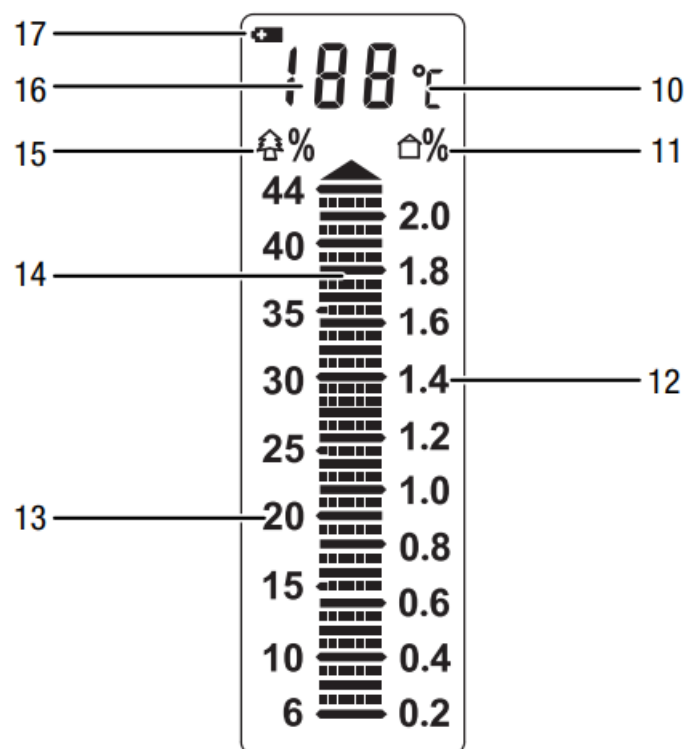

No.	Designation
10	°C / °F indication
11	Indication of the building moisture measuring mode
12	Numeric values for building moisture measurement
13	Numeric values for wood moisture measurement
14	Measured value scale (1 bar corresponds to 1 % of wood moisture or 0.05 % of building moisture)
15	Indication of the wood moisture measuring mode
16	Measurement value indication
17	Battery indication

Technical data

Measuring principle:	resistance measuring method
Dimensions:	145 x 44 x 34 mm
Weight:	132 g (incl. batteries)
Measuring range:	Wood moisture: 6 to 44 % Building moisture: 0.2 to 2.0 % Temperature: 0 to 40 °C (32 to 104 °F)
Measuring range resolution:	Wood moisture: 1 % Building moisture: 0.05 % Temperature: 1 °C (2 °F)
Accuracy:	Wood moisture measured value until 30 %: ± 2 % Wood moisture measured value from 30 %: ± 4 % Building moisture measured value until 1.4 %: ± 0.1 % Building moisture measured value from 1.4 %: ± 0.2 % Temperature: not specified
Ambient temperature:	0 to 50 °C with 0 to 85 % RH
Power supply:	4 x 1.5 V batteries AAA
Automatic switch-off:	after approx. 30 seconds

Scope of delivery

- 1 x Moisture measuring device BM22
- 4 x AAA batteries
- 1 x Quick guide

Transport and storage

Note

If you store or transport the device improperly, the device may be damaged. the information regarding transport and storage of the device.

Transport

For transporting the device, use the bag included in the scope of delivery in order to protect the device from external influences.

Storage

When the device is not being used, observe the following storage conditions:

- dry and protected from frost and heat
- protected from dust and direct sunlight
- with a cover to protect it from invasive dust if necessary
- the storage temperature complies with the values specified in the Technical data
- Remove the batteries from the device.


Operation

Inserting the batteries

Insert the supplied batteries before first use.

Note

Make sure that the surface of the device is dry and the device is switched off.

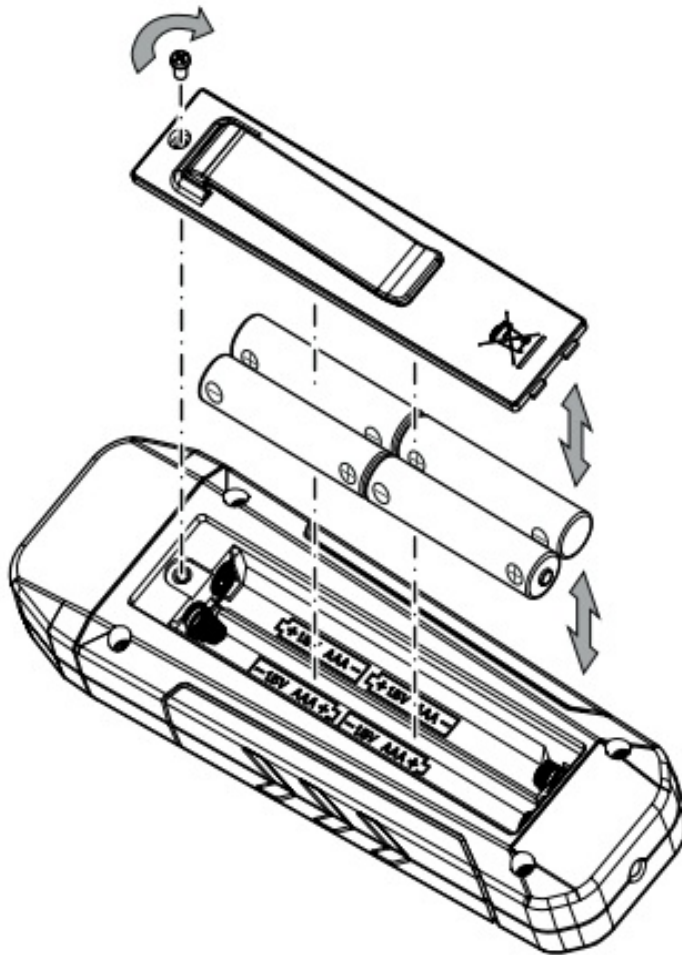

1. Unscrew the screw from the battery compartment.
2. Remove the cover from the device.
3. Insert the new batteries in the compartment with the correct polarity.
4. Fit the cover back on the device.
5. Tighten the screw.
6. Switching the device on

Info

Please note that moving from a cold area to a warm area can lead to condensation forming on the device's circuit board. This physical and unavoidable effect can falsify the measurement. In this case, the display shows either no measured values or they are incorrect. Wait a few minutes until the device has become adjusted to the changed conditions before carrying out a measurement.


1. Press the SET/ON button (6).

The display switches on.

The device is ready for operation.

Performing a function test

1. Hold the measuring tips to the contacts lettered -T- at the top of the protective cap (device test).
The scale ought to indicate the value 19 % \pm 1.
 2. Hold the measuring tips to the contacts lettered -B- at the top of the protective cap (battery test).
All scale bars (14) should be flashing.
- If the device reacts as described, the general function test is completed with a positive result.

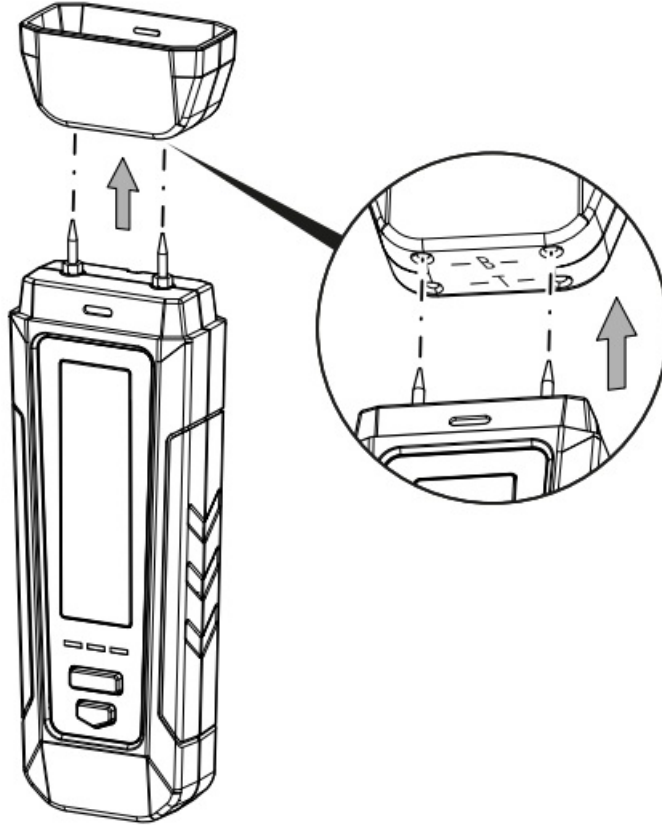

If the device does not react as described, please check the battery voltage or replace the batteries with new ones of high quality. If this does not solve the problem, please contact the Trotec customer service.

Measuring temperature

The ambient temperature determined by the device is indicated on the display (16) in real time.

Moisture measurement

1. Remove the protective cap.
2. If possible, carefully prick the measuring tips a few millimetres into the material.
When measuring wood moisture, read the measured value off the left-hand side of the scale (13).
When measuring building moisture, read the measured value off the right-hand side of the scale (12).
3. Carefully pull the device out of the material by gently moving it in turns to the left and to the right.
4. Upon conclusion of the measurement put the protective cap back on the device.

Reading the LED display

In the wood moisture measuring mode the LEDs are to be read as follows:

- At a measured wood moisture of less than 6 % none of the LEDs is illuminated.

- At a measured wood moisture between 6 % and 16 % the green LED is illuminated.
- At a measured wood moisture between 16 % and 20 % the yellow LED is illuminated.
- At a measured wood moisture of more than 20 % the red LED is illuminated.

In the building moisture measuring mode the LEDs are to be read as follows:

- At a measured building moisture of less than 0.2 % none of the LEDs is illuminated.
- At a measured building moisture between 0.2 % and 0.7 % the green LED is illuminated.
- At a measured building moisture between 0.7 % and 0.9 % the yellow LED is illuminated.
- At a measured building moisture of more than 0.9 % the red LED is illuminated.

Changing the unit °C / °F

1. Press the SET/ON button (6) for approx. 3 seconds.

The display (10) changes to either °C or °F.

The measured value adapts to the selected unit.

Switching on the LED illumination

1. Press the Lamp button (5) for approx. 3 seconds to switch on the LED illumination (4).

Press the Lamp button (5) for approx. 1 second to switch the LED illumination (4) back off.

Switching the device off

The device switches off after approx. 30 seconds without being used.

Info

Please bear in mind that with activated LED illumination the device will NOT switch off automatically. Switch off the LED illumination as formerly described.

Measuring principle

The measuring device at hand serves for the rough determination of the material or wood moisture content according to the resistance measuring method. Fields of application are wood moisture measurements of sawn timber and firewood. Moreover, the measuring device can be used to detect moisture in soft building materials such as gypsum or plaster. The resistance measuring method is an indirect measurement method since the moisture content of the measured material is deduced from its conductivity. Influencing variables suitable to change the conductivity, e.g. electrically conducting materials or dissolved salts, hence also have a direct influence on the determined measured values. Therefore, the displayed measured values can only be considered as indicators of the moisture content.

Notes on use regarding the wood moisture measurement:

For wood moisture measurement a calibration curve is stored in the device, which corresponds to the average of the relevant kinds of wood in Europe based on a wood temperature of 20 °C. Therefore, no further settings are required for a quick rough determination of the wood moisture content. If precise wood moisture values are required for other wood temperatures or with due regard of the type and bulk density of certain timber, an additional control measurement applying the Darr procedure or else using wood moisture measuring device with temperature comparison function and selection option for the specific wood type calibration is recommended.

- Always insert the measuring tips transverse to the wood fibre direction. The conductivity transverse to the

wood fibre direction is lower than that in line with it.

- When selecting the measuring positions observe the following:
 - Always measure the material moisture at at least three different positions in order to achieve sufficient accuracy by means of the arithmetic average.
 - Do not measure the face, because there are mainly dry areas.
 - Preferably do not measure at cracks, branches or resin pockets either.
- Oily and/or aqueous timber preservatives affect the measurement result.
- If possible, do not measure wood with a temperature below -5 °C. Too low wood temperatures distort the result of the measurement.
- Avoid static charge of the material to be measured due to friction. Static charge distorts the measurement result.
- With a wood moisture of less than 10 % RH, electrostatic forces may occur at the good to be measured. This can falsify the result of the measurement. Experience has shown that this occurs at the outlet of veneer drying plants. Remove the static charge by use of suitable grounding measures.
- The measurement's accuracy depends on the contact pressure of the measuring tips. The measuring tips must be connected to the wood in a way that the contact resistance is small as compared to the measuring resistance.

Notes on use regarding the material moisture measurement:

- When assessing the measurement results one has to bear in mind that increased occurrences of soluble salts in the measured material can distort the result of the measurement. The more salts present, the higher the conductivity
- of the material and the higher will be the displayed measurement value.
- Further observe disruptive influences due to electrically conducting substances:
- If a construction material contains electrically conducting substances, it also has a lower resistance value, which then simulates high moisture values. Consequently, a too high measured value will be displayed.
- From visual inspection it is not always apparent, whether there are any electrically conducting substances inside the construction material.
- Some of the main error sources here are in particular reinforcements, metal laminations and conducting insulation such as slag in timber beam ceiling constructions. Especially in case of insulation materials with metal lamination,
- measured values are often misinterpreted during the resistance measurement. Quantitative conclusions about the moisture content of the mineral material to be measured can only be drawn by applying the Darr procedure or the CM method.


Maintenance and repair

Exchanging measuring tips


Exchange the measuring tips when these exhibit signs of wear (e.g. oxidation, deformation, heavy, irremovable contamination).

Ensure that the device is switched off.


1. Remove the protective cap from the device.

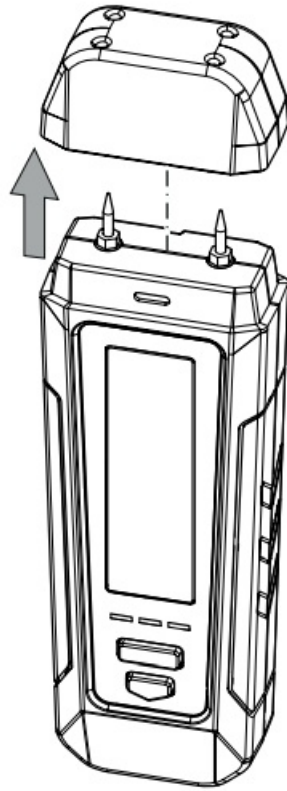

2. Detach the screwed-on measuring tips from the device.

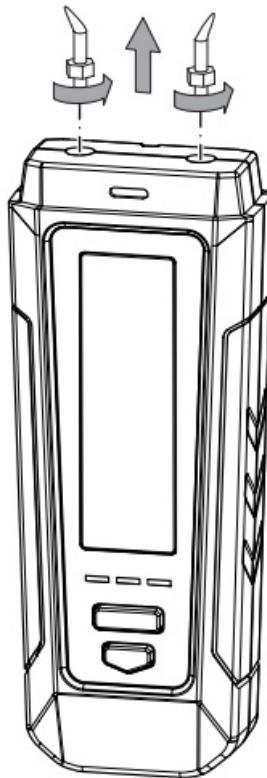

3. Screw the new measuring tips into the device.

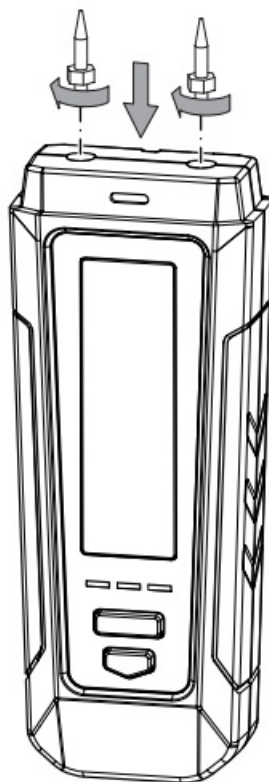

Cleaning

Clean the device with a soft, damp and lint-free cloth. Make sure that no moisture enters the housing. Do not use any sprays, solvents, alcohol-based cleaning agents or abrasive cleaners, but only clean water to moisten the cloth.

Repair

Do not modify the device or install any spare parts. For repairs or device testing, contact the manufacturer.

Errors and faults

Fault	Remedy
Display segments are only faintly visible or flicker.	The battery voltage is too low. Exchange the batteries immediately.
The device displays implausible measured values.	

The device has been checked for proper functioning several times during production. If malfunctions occur nonetheless, check the device according to the following list.


Disposal

- The icon with the crossed-out waste bin on waste electrical or electronic equipment stipulates that this equipment must not be disposed of with the household waste at the end of its life. You will find collection points for free
- return of waste electrical and electronic equipment in your vicinity. The addresses can be obtained from your municipality or local administration. You can also find out about other return options that apply for many EU
- countries on the website <https://hub.trotec.com/?id=45090>. Otherwise, please contact an official recycling centre for electronic and electrical equipment authorised for your country.
- The separate collection of waste electrical and electronic equipment aims to enable the re-use, recycling and

other forms of recovery of waste equipment as well as to prevent negative effects for the environment and human

- health caused by the disposal of hazardous substances potentially contained in the equipment.
- In the European Union, batteries and accumulators must not be treated as domestic waste, but must be disposed of professionally in accordance with Directive 2006/66/EC of the European Parliament and of the Council of
- 6 September 2006 on batteries and accumulators. Please dispose of batteries and accumulators according to the relevant legal requirements.
- **Only for United Kingdom**
- According to Waste Electrical and Electronic Equipment Regulations 2013 (2013/3113) and the Waste Batteries and Accumulators Regulations 2009 (2009/890), devices that are no longer usable must be collected separately and disposed of in an environmentally friendly manner.

Documents / Resources

	<p>TROTEC BM22 Moisture Measuring Device [pdf] User Manual BM22 Moisture Measuring Device, BM22, Moisture Measuring Device</p>
--	--