



VIVE LEG Compression System RHB1019 Owner's Manual

[Home](#) » [Vive](#) » VIVE LEG Compression System RHB1019 Owner's Manual 

vive®



LEG COMPRESSION SYSTEM
Owner's Manual RHB1019

Contents

- 1 OVERVIEW
- 2 QUICK START GUIDE
- 3 MESSAGE MODES: THREE SET MODES
- 4 HOW TO USE THE LEG CUFF
EXTENDERS
- 5 CLEANING AND MAINTENANCE
- 6 PUMP SPECIFICATIONS
- 7 Documents / Resources
- 8 Related Posts

OVERVIEW

We are constantly answering questions and recording helpful videos to make using your Vive Leg Compression System as easy as possible. Check out the included links and QR codes to help you through the process.



To see all of the FAQs in one place, visit vhealth.link/g9m

QUICK START GUIDE



For a video demonstration on how to use your Leg Compression System, visit vhealth.link/2oq

Note: For first-time use, open the filter cover and remove the screw!

1. Turn pump over. Open-air filter and remove plug screw.
2. Connect the power cord to a power outlet.
3. Securely connect the air hose to the pump.
4. Connect the air hose to the leg cuff.

Note: Longest air hose connects to the uppermost air valve.


5. Press the power button.
6. Select the desired pressure using the pressure control.
7. Set the inflate and deflate times as desired.

MASSAGE MODES: THREE SET MODES

A: In this mode, only a single chamber is inflated at a time. Starting from the toes and working up to the thigh. Then the cycle repeats. Ideal for massage.



B: In this mode, the toe chamber stays inflated. It gradually adds a chamber until all four are filled with air. Then the cycle repeats. Ideal for lymphatic edema treatment.

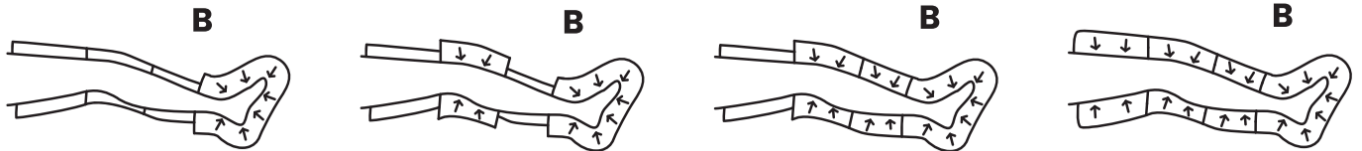


C: In this mode, every other chamber is inflated. This is great for massage and post-workout recovery.



HOW TO USE THE LEG CUFF EXTENDERS

The Vive Leg Compression System comes with a pair of leg cuff extenders that increase the circumference of the cuff up to 4 inches, providing a better fit for larger or swollen legs.

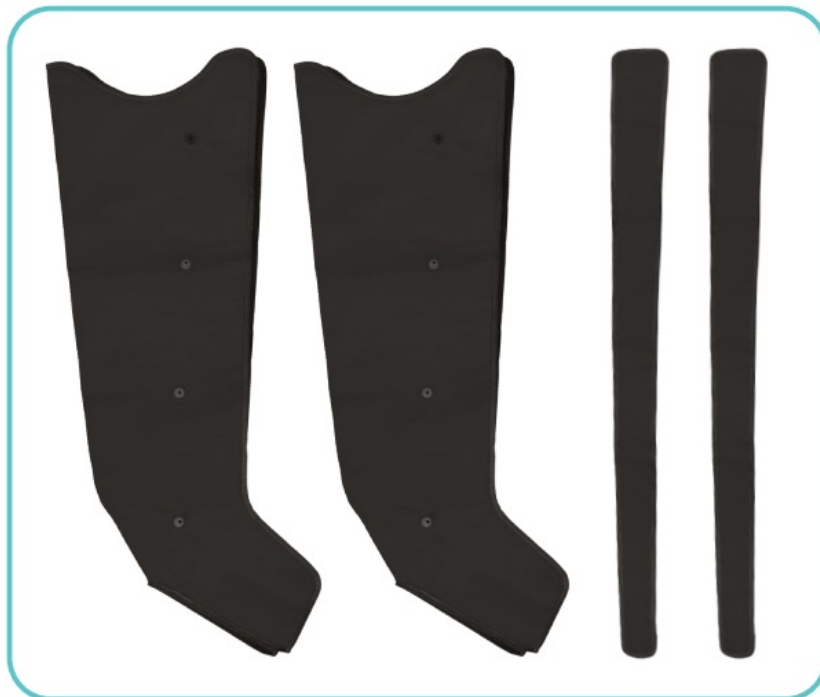

To attach the extenders, use the zipper slider and insertion pin from the extenders to secure onto the main cuff.



Note: The extender should be attached with the wider part at the top.

CLEANING AND MAINTENANCE

- Turn off the pump before cleaning.
- Wipe with a damp cloth.

WARNING

- Do not unzip the garment when the unit is on.
- Always turn the power off before unzipping the cuff.
- Do not get the pump wet
- Make sure the pump is on a flat surface.

PUMP SPECIFICATIONS

- Power Consumption: 30 W
- Input Voltage: 110 V
- Pressure Range: 30-250mmhg

Documents / Resources



[VIVE LEG Compression System RHB1019](#) [pdf] Owner's Manual
VIVE, LEG Compression System, RHB1019