



ziso M3 Infrared Electronic Thermometer User Guide

[Home](#) » [ziso](#) » ziso M3 Infrared Electronic Thermometer User Guide 


ziso M3 Infrared Electronic Thermometer



Contents

- [1 Introduction](#)
- [2 Specification](#)
- [3 Status Description](#)
- [4 Operation Instruction](#)
- [5 Documents / Resources](#)
- [6 Related Posts](#)

Introduction

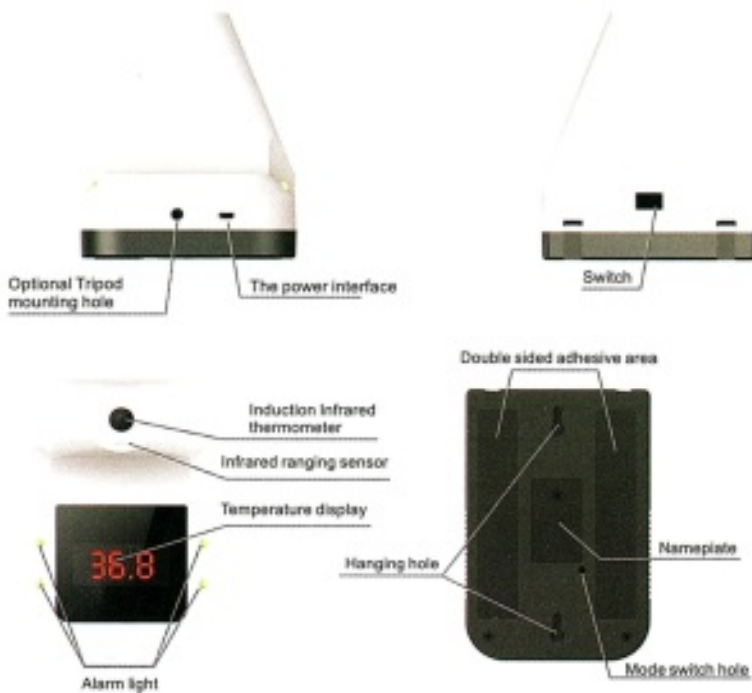

Specification

1. **Accuracy:** ± 0.2 degrees ($34 - 45^{\circ}\text{C}$, place it in the operating environment for 30 minutes before use)
2. **Abnormal automatic alarm:** flashing + “Di Di” sound
3. **Automatic measurement:** measuring distance 5cm -10cm
4. **Screen:** Digital display
5. **Charging method:** USB charging or battery(18650 Li- ion).
6. **Install method:** nail hook (optional), double-sided adhesive sticking, bracket fixing(optional)
7. **Environment temperature:** 10°C - 40°C (Recommended 15°C ~ 35°C)
8. **Infrared measuring range:** $0 - 50^{\circ}\text{C}$
9. **Response time:** 0.5s
10. **Input:** DC 5V
11. **Net weight:** 350g
12. **Dimension:** 170* 115* 140mm
13. **Standby:** About one week
14. **Counting capacity:** 999

Status Description

1. Standby. The red dot in the bottom of the display lights up in turn. **(Fig.1)**

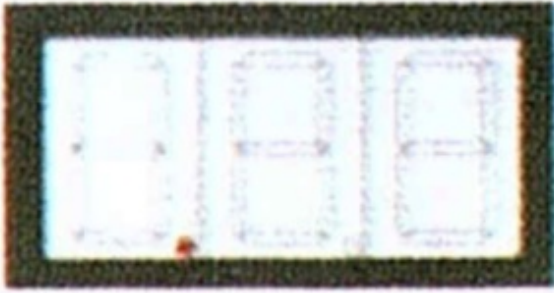


Fig. 1

2. Insufficient power: The horizontal bar lights up in the middle of the display. **(Fig. 2)**

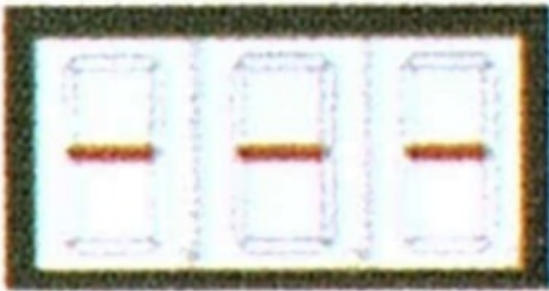


Fig. 2

3. Normal temperature: Flashing green lights and alarm “Di”. **(Fig. 3)**



Fig. 3

4. Abnormal temperature: Flashing red lights and alarm “Di Di”. **(Fig 4)**



Fig. 4

5. Default (bod object mode)

“Lo”: Ultra-low temperature alarm. (Fig. 5)



Fig. 5

“HI”: Ultra-high temperature alarm. (Fig .6)



Fig. 6

Operation Instruction

1. Temperature measurement: Front of the thermometer and approach it within 5-10 cm. (Fig 7)

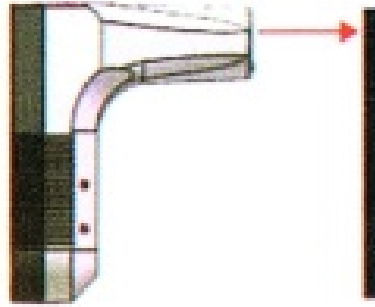


Fig. 7

2. Mode switching : There is a small hole on the back of the device (**Fig. 8**).

You can use a 3mm diameter screwdriver to insert the hole and then press the button.

(1) Temperature unit: Press 'mode switch hole' then select "C" or "F" (**Fig.9, 10**) C: Celsius F: Fahrenheit



Fig. 8



Fig. 9



Fig. 10

(2) Mode: Long press mode switch hole for 3 seconds to switch the temperature measurement mode (Sur: surface mode, bod: object mode, Cou: counting mode)



Fig.11



Fig.12



Fig.13

3. install and replace battery

(1) Remove three screws


(2) Open the back base and install 18650 Li battery




4. install method



1.Nail hook




2.Bracket fixing



3.Double-sided adhesive sticking

Documents / Resources



[ziso M3 Infrared Electronic Thermometer](#) [pdf] User Guide

M3, Infrared Electronic Thermometer, M3 Infrared Electronic Thermometer, Electronic Thermometer